

Received August 17, 2019, accepted September 7, 2019, date of publication September 16, 2019,  
date of current version September 26, 2019.

Digital Object Identifier 10.1109/ACCESS.2019.2941491

# Artificial Muscle Intelligence System With Deep Learning for Post-Stroke Assistance and Rehabilitation

SUNIL JACOB<sup>1,2</sup>, VARUN G. MENON<sup>1,3</sup>, FADI AL-TURJMAN<sup>1,4</sup>, (Member, IEEE), VINOJ P. G.<sup>2,5</sup>,  
AND LEONARDO MOSTARDA<sup>1,6</sup>

<sup>1</sup>Center for Robotics, SCMS School of Engineering and Technology, Ernakulam 683576, India

<sup>2</sup>Department of Electronics and Communication Engineering, SCMS School of Engineering and Technology, Ernakulam 683576, India

<sup>3</sup>Department of Computer Science and Engineering, SCMS School of Engineering and Technology, Ernakulam 683576, India

<sup>4</sup>Computer Engineering Department, Antalya Bilim University, 07190 Antalya, Turkey

<sup>5</sup>Department of Electronics and Communication Engineering, APJ Abdul Kalam Technological University, Thiruvananthapuram 695016, India

<sup>6</sup>Computer Science Division, University of Camerino, 62032 Camerino, Italy

Corresponding author: Varun G. Menon (varunmenon@scmsgroup.org)

This work was supported by The Institute of Electrical and Electronics Engineers (IEEE) EPICS, USA, under Grant 2016-12.

**ABSTRACT** Stroke is one of the prime reasons for paralysis throughout the world caused due to impaired nervous system and resulting in disability to move the affected body parts. Rehabilitation is the natural remedy for recovering from paralysis and enhancing the quality of life. Brain Computer Interface (BCI) controlled assistive technology is the new paradigm, providing assistance and rehabilitation for the paralysed. But, most of these devices are error prone and also hard to get continuous control because of the dynamic nature of the brain signals. Moreover, existing devices like exoskeletons brings additional burden on the patient and the caregivers and also results in mental fatigue and frustration. To solve these issues Artificial Muscle Intelligence with Deep Learning (AMIDL) system is proposed in this paper. AMIDL integrates user intentions with artificial muscle movements in an efficient way to improve the performance. Human thoughts captured using Electroencephalogram (EEG) sensors are transformed into body movements, by utilising microcontroller and Transcutaneous Electrical Nerve Stimulation (TENS) device. EEG signals are subjected to pre-processing, feature extraction and classification, before being passed on to the affected body part. The received EEG signal is correlated with the recorded artificial muscle movements. If the captured EEG signal falls below the desired level, the affected body part will be stimulated by the recorded artificial muscle movements. The system also provides a feature for communicating human intentions as alert message to caregivers, in case of emergency situations. This is achieved by offline training of specific gesture and online gesture recognition algorithm. The recognised gesture is transformed into speech, thus enabling the paralysed to express their feelings to the relatives or friends. Experiments were carried out with the aid of healthy and paralysed subjects. The AMIDL system helped to reduce mental fatigue, miss-operation, frustration and provided continuous control. The thrust of lifting the exoskeleton is also reduced by using light weight wireless electrodes. The proposed system will be a great communication aid for paralysed to express their thoughts and feelings with dear and near ones, thereby enhancing the quality of life.

**INDEX TERMS** Artificial muscle intelligence, assistivetechologies, BCI, EEG, exoskeleton, healthcare, intelligent solutions, deep learning system, paralyzed, stroke.

## I. INTRODUCTION

The recent survey by reeve foundation revealed the impact of paralysis on world population, affecting approximately 5.4 million people [1], [2]. The survey also identified stroke (33.7%) as the major cause for paralysis. Paralysis is the deficiency of brain to activate muscle function of any body

The associate editor coordinating the review of this manuscript and approving it for publication was Shadi Aljawarneh.

part. Paralyzed persons find it difficult to perform their routine activities without assistance. Rehabilitation is one of the natural ways of healing paralysis. Because of this there is increasing interest and involvement in the field of post stroke rehabilitation. Exoskeleton-assisted technologies have emerged as a reliable means for rehabilitation of the affected upper and lower limbs [3]. Exoskeleton movements were controlled using sensors like gyroscopes, accelerometers, and potentiometers. Recently the focus is on controlling

exoskeleton using Brain Computer Interface (BCI) [4]. Antelis *et al.* demonstrated upper limb movement of the paralyzed using EEG signals [5]. A closed loop is established between human thought and movement of paralyzed limb using non-invasive BCI [6]. Android feedback based BCI training is employed to enhance brain rhythms during motor imagery task. The realistic feedback is realized in training session using humanoid robot [7]. Humanoid robot is navigated in real-time indoor environment based on human intentions. The asynchronous BCI system was designed using two level classifiers [8]. Co-operation and co-ordination of dual robotic arm is demonstrated using EEG based system. SSVEP (Steady-State Visual Evoked Potentials) are utilized to improve the user concentration level [9]. Electromyography (EMG) sensors are also used to control exoskeleton movements, EMG returns the information regarding human muscular activity [10]. The motor adaptability of upper limb is predicted using resting state functional connectivity. The system could identify effectiveness of robotic upper limb rehabilitation in different patients [11]. However, the system does not investigate real time human behaviors and thoughts. The clinical trials to investigate the effectiveness of BCI training sessions on stroke patients with upper limb paralysis are carried out. The results of the trial indicate that BCI based assistive devices are effective for post stroke rehabilitation [12]. Human intentions measured through cortical potentials were used to control upper-limb exoskeleton movements. The BMI system eliminated the need for recalibration but resulted in large false positive rates [13]. Grasping feature is incorporated into the assistive device for amputees using non-invasive EEG control. The participants were able to grasp the objects, but resulted in low success rate without sufficient training [14]. Brain activity is modulated to control robotic arm with multiple degrees of freedom. The system demonstrated the effective control of robotic arm with few training sessions, but increased the latency periods during certain operations [15]. Hybrid BMI system based on sensorimotor cortical desynchronization (ERD) and electromyography (EMG) activity was designed to control upper limb movements. The integration of BMI, NMES and exoskeleton improved the system accuracy, but increased the system complexity [16]. The linear control of upper limb is demonstrated using motor imagery based BCI and Functional Electrical Stimulation (FES), support is provided to the arm using passive exoskeleton. The generated limb movement is evaluated to identify the precise positioning [17]. The self-induced EEG variations based on ERD/ERS is utilized for controlling upper limb movements. Distinguishable patterns are obtained for left and right-hand movements in both motor imagery and motor execution experiments [18]. Online robot control using motor imagery based BCI is designed with high classification accuracy. The mental imagination of hand movement is detected for controlling the robot movements [19]. An integrated platform consisting of BCI controlled exoskeleton, functional electric stimulation (FES) with proprioceptive feedback is developed. Goal directed

motor task is used for training and subjects could complete the task with minimum latency period [20].

In our previous works [21]–[23], we have demonstrated an alternative technology to exoskeletons using non-invasive brain signals. Also, exoskeletons with feedback mechanism has also been implemented by us [22]. The paralyzed body part is stimulated using Transcutaneous Electrical Nerve Stimulation (TENS) device and Microcontroller [24]. Because of the dynamic and uncertain nature of brain signals, most of the BCI systems result in miss-operation, mental fatigue and it is hard to produce continuous control. The proposed system is designed to address the above gaps in research.

AMIDL is designed to reduce miss-operation, user fatigue and to enhance user capabilities. In the proposed work, human intentions are monitored in real-time employing 16 channel EEG sensors. TENS machine is integrated with Muscle Inspired Algorithm (MIA) to produce movements on the upper limb. Subjects are relieved from the task of carrying exoskeleton structure. The system is designed to perform six different movements on the affected upper limb. The different hand postures used to trigger the rehabilitation process are Release, Grasp, Rollup, Roll down, Rollup Release and Rollup grab. In the offline phase, Artificial Muscle movements corresponding to each posture are recorded to create the database. The decoded EEG signals are transformed into muscle activation signals in real-time environment. The captured EEG signal is converted into frequency domain using Walsh Hadamard Transform (WHT) for feature extraction. The extracted features along with WHT coefficients are utilized for the classification of different limb movements. The activation signal is then correlated with the recorded muscle movements. The signal with superior characteristics is passed on to the upper limb electrodes for inducing motion. In case of ambiguity or inadequate EEG signal, the periodic activation of the affected body part will be taken care by the artificial muscle movements. If the activation is executed by brain signal, the produced gesture is recognized and passed on to the care giver as voice command. Thus, AMIDL transforms human thoughts into different movements on the unique upper limb structure. The EEG activated movements are utilized for communicating paralyzed person's emergency need to the caregivers.

The contributions of our research are,

- An Artificial Muscle Intelligence with Deep Learning (AMIDL) system without exoskeleton structure, in which movements of paralyzed body part is controlled based on user intentions.
- An adaptive mechanism based on recorded muscle movements is integrated with the system to enhance continuous control and facilitate rehabilitation.
- Designed flexible assembly, which can be customized according to the degree of disability.
- Communication aid is incorporated in the system using gesture recognition

- The subject concentration is improved by using multi-media feed back

The rest of the paper is organized into four sections in which section 2 describes different existing methods used in BCI controlled upper limb movements.

## II. RELATED WORKS

In this section, we discuss few existing devices controlled by Brain-Computer Interface designed specifically for paralyzed people. But the problem with most of them is that the users are unable to get continuous control over the device. The users are required to have high level of concentration to get sufficient control on the device, which results in mental fatigue and frustration. Additionally, there is no arrangement to take care of the miss-operations. The subjects are also burdened with the task of carrying the load of exoskeleton on the affected body parts. Our research focus on overcoming these major problems and provides an efficient and flexible solution, which can enhance the post stroke recovery process. Our system also provides a communication aid for the paralyzed to express their feelings.

The assistive rehabilitation devices and its EEG control techniques are systematically reviewed and the major gaps are identified [25]. Three-dimensional robotic assistance using motor imagery task for upper limb rehabilitation is demonstrated with multi-joint exoskeleton. Desynchronization of sensorimotor oscillations in the  $\beta$ -band is measured to control the different robotic hand movements [26]. Different upper limb exoskeletons like Track hold [27] and Armeospring [28] are employed to track upper limb movements. Both these devices have integrated passive robots with virtual reality environment to help patients carry out their daily routine activities. Control of assistive robots are improved by integrating electroencephalography (EEG) and electrooculography (EOG). This hybrid approach called as brain/neural-computer interaction (BNCI) is adopted to control grasping movements of a hand exoskeleton [29]. Multimodal signal approach is further used to enhance control system for external device connected to the upper limb. EEG and EMG signals are integrated to improve the classification accuracy and to reduce the false positive rate [30]. Upper limb robotic orthosis, FES, and wireless BCI are combined in an efficient way on account of EEG signals. EMOTIV EEG device is employed to measure EEG signal, which is used to control grasp/release of an object [31]. An integrated passive robotic system is developed for assisting the paralyzed. The system employs a robotic device which compensates gravitational effects to allow exercise, virtual engines to facilitate interaction and EEG to monitor brain activities. The three components are coordinated in real-time to enhance the rehabilitation process [32]. The effects of BCI therapy on post stroke rehabilitation is analyzed based on motor imagery tasks. The analysis is performed by measuring coherence of EEG in different regions of the brain and the best result for motor recovery is obtained for the activation of lesion hemisphere [33]. The online BCI coupled with hand exoskeleton

is employed to address the issues related to proprioceptive feedback on the regulation of cortical oscillations. The results show an enhancement in SMR desynchronization with proprioceptive feedback during flexing and extending fingers of the exoskeleton [34]. Multimodal architecture based on BCI, exoskeleton and an active vision system is proposed to enhance BCI control and rehabilitation process. The VR environment coupled with bio feedback help to reduce mental fatigue and improve user interactions [35]. Few studies have also been conducted in related areas recently [36]–[42]. Al-Turjman *et al.* proposed another interesting system using optimal haptic communications [43]. Xu *et al.* [44] proposed a three-dimensional animation to guide upper limb movements using EEG signals. Feature extraction is carried out by Harmonic Wavelet Transform (HWT) and linear discriminant analysis (LDA) classifier was utilized to classify the patterns for controlling the upper limb movements. MR-compatible robotic glove operates pneumatically and doesn't cause any disturbance to functional Magnetic Resonance imaging (fMRI) images during rehabilitation process [45]. The resistance to mechanically actuated movements in exoskeleton robot is measured based on spasticity. The relevant guidelines for practical neuro-rehabilitation robot design based on degree of spasticity and resistance is established [46]. In most of the design it is hard to get continuous control on the exoskeleton due to the non-stationary nature of the EEG signal. Moreover, the subjects experience metal fatigue and frustration due to lack of superior control. None of the device in the literature focused on providing communication aid for the paralyzed. Our research focus on solving these issues in an efficient manner using AMIDL system proposed in this paper. Table 1 shows the comparisons between AMIDL and existing systems in the literature.

## III. MATHEMATICAL MODEL

This section presents and discusses the mathematical modelling of the proposed system. The system is designed to perform six different movements on the affected upper limb. The different hand postures used to trigger the rehabilitation process are Release, Grasp, Rollup, Roll down, Rollup Release and Rollup grab. In the offline phase, Artificial Muscle movements corresponding to each posture are recorded to create the database. The decoded EEG signals are transformed into muscle activation signals in real-time environment.

In Hand Posture Release operation, the voltage and current applied to electrodes are assumed as  $V_{H-P-R}$  &  $I_{H-P-R}$ . Similarly, the voltage and current applied to electrodes in the other postures are defined as,

$$\text{Hand Posture Release} \rightarrow V_{H-P-R} I_{H-P-R}$$

$$\text{Hand Posture Grasp} \rightarrow V_{H-P-G} I_{H-P-G}$$

$$\text{Hand Posture Roll up} \rightarrow V_{H-P-Ru} I_{H-P-Ru}$$

$$\text{Hand Posture Roll down} \rightarrow V_{H-P-Rd} I_{H-P-Rd}$$

$$\text{Hand Posture Role up Release} \rightarrow V_{H-P-R-R} I_{H-P-R-R}$$

$$\text{Hand Posture Roll up Grasp} \rightarrow V_{H-P-R-G} I_{H-P-R-G}$$

The voltage for Hand Posture Release,  $V_{H-P-R} \neq$  Hand Posture Grasp,  $V_{H-P-G}$ . If they are same the hand posture

**TABLE 1. AMIDL comparisons with existing system (Sorted by success rate).**

METHOD REFERENCE NO., YEAR	NO. OF SUBJECTS	TYPE OF CONTROL	TYPE OF EEG SIGNAL	DEVICE ASSIGNED	TASK	ACCURACY/SUCCESS RATE
Ref [14], 2016	2 amputees	EEG -based control	Motor imagery Low frequency-time domain feature	Prosthetic hand	Grasping objects	63.6%
Ref [15], 2016	13 healthy subjects	EEG-based control	ERD/ERS	Arm exoskeleton	Reach and grasp tasks	77.8%
Ref [12], 2017	64 stroke patients	EEG-based control	Motor imagery 5–30 Hz EEG signal	Hand exoskeleton	Hand open/closed	79.4%
Ref [17], 2016	7 healthy subjects	EEG-based control	7–30 Hz EEG signal	ArmeoSpring and FES	left hand, right hand, and feet	79.6%
Ref [16], 2016	7 stroke patients	EEG-based control	ERD	ArmeoSpring exoskeleton	Wrist extensor/flexor	80.7%
Ref [13], 2016	3 chronic stroke patients	EEG-based control	MRCPs	MAHI exoskeleton	Elbow flexion/extension	81.3%
Ref [11], 2018	19 healthy subjects	EEG-based control	15–25 Hz EEG signals	Robotic Arm	Upper limb movement/reaching	83.5%
Ref [18], 2016	4 healthy subjects	EEG-based control	ERD/ERS	Custom upper limb exoskeleton	Left/right hand and left hand versus both feet	84.29%
Proposed System, AMIDL	20 subjects	EEG and EMG based control	Motor Imagery ERD/ERS with multimedia feed back	TENS device with EMG Electrodes	left or right hand movements	87%

will be stable. If  $V_{H-P-R} > V_{H-P-G}$ , then Hand Posture Release will be activated compared to Hand Posture Grasp.

The other parameters in the system is defined as follows. The diameter of EEG electrode is  $D_E$ . The scalp resistance is  $S_R$ . The conductivity of the EEG electrodes depends upon the multiplying factor is assumed as ‘T’.

When the multiplying factor ‘T’ is more, the conductivity will be more & vice versa. The multiplying factor depends on the positioning of EEG electrodes, the diameter of EEG electrodes and scalp resistance.

The  $V_{H-P-T}$  denotes the Hand Posture Threshold. The threshold varies depending on the different types of postures.

**A. THE POSTER ACTIVATION REGION**

The Hand Posture Current in the system is given by,

$$I_{H-P} = \frac{D_E}{S_R} \int_{V_{H-P-initial}}^{V_{H-P-final}} T(E_Q) dV_{initial-final} \quad (1)$$

For the condition from Hand Posture Grasp to Hand Posture Release with the Hand Posture Threshold acting as an intermediate, the Hand Posture Release current is given by,

$$I_{H-P-R} = \frac{D_E}{S_R} \int_{V_{H-P-G}}^{V_{H-P-R}} T(E_Q) dV_{R-G} \quad (2)$$

where  $E_Q$  is the net potential to EEG electrodes. Also, we have,

$$E_Q = V_{H-P-R} - V_{H-P-T} - V_{H-P-G} \quad (3)$$

If  $E_Q$  is positive then,  $V_{H-P-R}$  is dominating  $V_{H-P-T}$  &  $V_{H-P-G}$ . The required potential to EEG electrodes will be analyzed and the Hand Posture Release operations will be performed.

For  $V_{H-P-G} < V_{H-P-T} \leq V_{H-P-R}$ , neglecting the surrounding areas of EEG electrodes and conductive loss. The hand posture for release will be activated as,

$$I_{H-P-R} = V_{H-P}(V_{H-P-G}, V_{H-P-R}) \quad (4)$$

Similar relation can be developed for the remaining postures.

If the movement is a combination of different postures, say Roll up and Release, then,

Let say the initial posture is in grasp stage,

$$I_{H-P-R-R} = \frac{D_E T}{S_R} \left\{ \int_{V_{H-P-G}}^{V_{H-P-Ru}} (V_{H-P-Ru} - V_{H-P-T} - V_{H-P-G}) dV_{G-Ru} + \int_{V_{H-P-Ru}}^{V_{H-P-R}} (V_{H-P-R} - V_{H-P-T} - V_{H-P-Ru}) dV_{Ru-R} \right\} \quad (5)$$

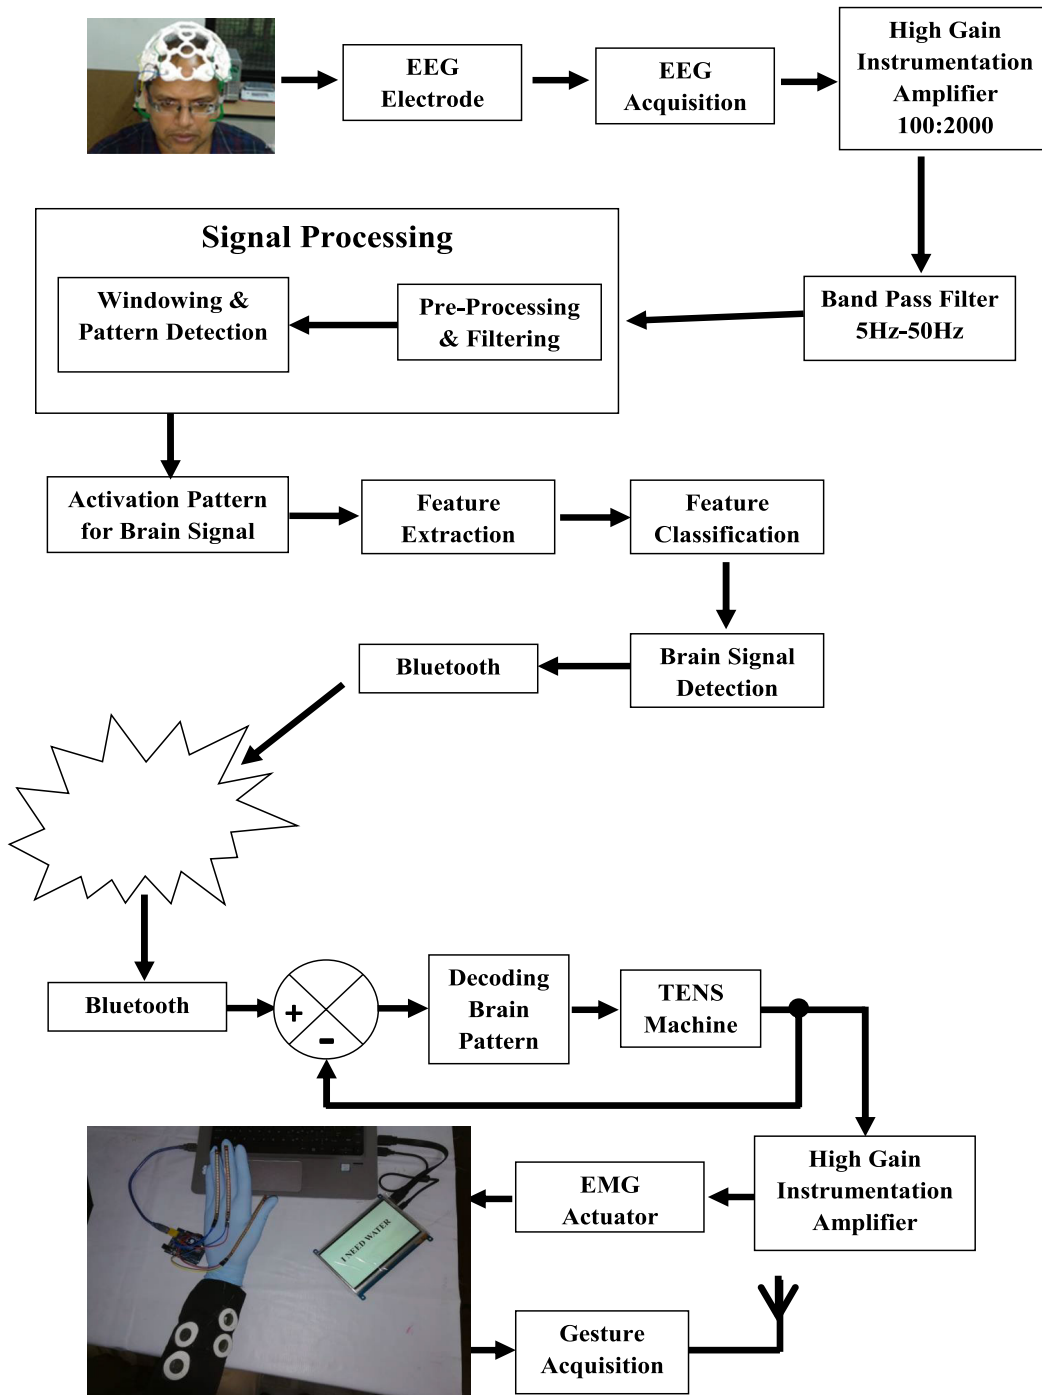


FIGURE 1. System architecture: AMIDL EEG acquisition and muscle stimulation modules.

Using the current value in the first integral and in the second integral we will have,

$$I_{H-P-R-R} = I_{H-P-G-Ru} (V_{H-P-G}, V_{H-P-G-Ru}) + I_{H-P-Ru-R} (V_{H-P-Ru}, V_{H-P-R}) \quad (6)$$

The mathematical model of the system can be summarized as  $I_{H-P}$ , as shown at bottom of the next page.

#### IV. SYSTEM ARCHITECTURE

The architecture of the proposed system is presented in figure 1.

##### A. AMIDL EEG ACQUISITION MODULE

The system architecture is designed using modular approach, it consists of three main modules. They are 1) EEG Acquisition Module, 2) Muscle Stimulation Module and



3) Gesture to Voice Conversion Module. Figure 1 indicates the two main modules of the system. The system captures brain signal using EEG sensor module, which has 14 electrodes to make measurement and two acts as reference. The acquired signal undergoes pre-processing, feature extraction and classification. The low amplitude EEG signal is amplified using high gain instrumentation amplifier with a gain of approximately 1000-2000 db. The signal is band limited by employing band pass filter having a pass band frequency of 5-50Hz. Windowing and pattern selection is utilized for getting finite response. Feature coefficients of the signal are extracted using Walsh Hadamard Transform (WHT). These extracted features are used to classify the thoughts into six different movements. The actual brain pattern is reconstructed using the transmitter Hadamard coefficients. The decoded brain pattern is given to the TENS device, which transforms the thought into muscular actions. The muscle inspired algorithm stored in the controller facilitates the process of conversion. In the offline phase, muscle movements correspond to the six different pre-defined hand postures are recorded to create the database. The hand postures are recorded using 7 Electromyography (EMG) sensors on the different hand muscles. Five EMG electrodes are placed on the finger muscles to record finger activity. Two electrodes are placed on either side of the elbow to identify roll movements. In the online phase, brain signal based on the human thought is acquired and transformed into muscle movement. This transformed muscle movement is then correlated with the recorded muscle movements. The signal with superior characteristics is selected by the controller for producing movements on the affected body part. If the brain signal fails to provide sufficient activation, periodic movements in the upper limb will be triggered by artificial muscle.

**B. AMIDL GESTURE TO VOICE CONVERSION MODULE**

If the brain signal with superior features activate the upper limb, the created gesture will be captured. Flex sensors placed on each finger is used for acquiring the gesture. The captured gesture will be recognized by the algorithm and transforms it into voice commands for the care givers. Figure 2 depicts the AMIDL gesture to voice conversion module. This module is used to give emergency alert messages to the caregivers or relatives.

The main hardware designed for the system has two parts 1) Acquisition module and 2) Muscle stimulation module. The brain signals of the user are acquired by using the EEG sensor. The non-invasive EEG sensor employed captures human intentions using 16 electrodes placed in the structure. 14 electrodes are used for capturing the signal and two electrodes act as reference. Figure 3 depicts the capturing of

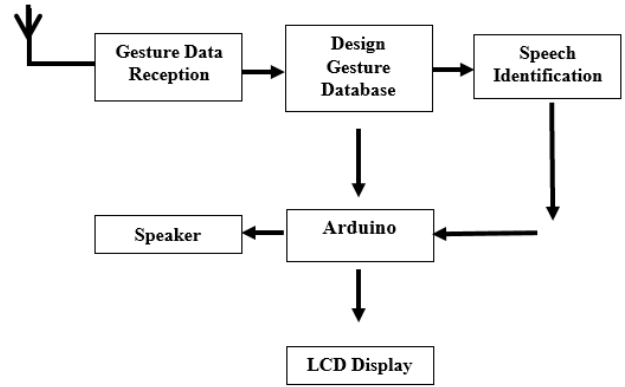


FIGURE 2. AMIDL gesture to voice conversion.



FIGURE 3. Signal acquisition using EEG sensor [21].

EEG signal using sensor from a human subject. The acquired signal is amplified using high gain instrumentation amplifier. The signal is band limited by employing band pass filter with pass band frequency in range of 5-50Hz

Signal undergoes further pre-processing and filtering to reduce the high frequency noise. Frequency domain conversion of the signal is done by using WHT transform and finite sample is selected using window technique. The design uses microcontroller in the acquisition and muscle stimulation module. The microcontrollers communicate with each other using Bluetooth technology. Bluetooth is selected because of short distance between modules and data rate required is less than 1mbps. EEG sensor and other electronic circuits are interfaced to the microcontroller to design the PCB. Figure 4 shows the electronic assembly used in our experimentation.

The muscle stimulation module receives the data using wireless module. The received data is converted into muscle movements or stimulation using muscle inspired algorithm stored in Arduino along with the TENS device interfaced to it. The output of the TENS is connected to the EMG electrode through EMG shield to activate the affected upper

$$I_{H-P} = \begin{cases} I_{H-P-R} (V_{H-P-G}, V_{H-P-R}) & \text{for } V_{H-P-G} < V_{H-P-T} \leq V_{H-P-R} \\ I_{H-P-G-Ru} (V_{H-P-G}, V_{H-P-Ru}) & \text{for } V_{H-P-G} < V_{H-P-T} \leq V_{H-P-Ru} \\ I_{H-P-Ru-R} (V_{H-P-Ru}, V_{H-P-R}) & \text{for } V_{H-P-Ru} < V_{H-P-T} \leq V_{H-P-R} \end{cases}$$

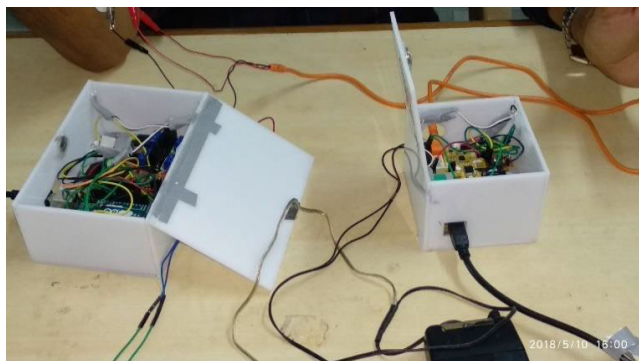


FIGURE 4. PCB designed for the experimentation.



FIGURE 5. Acquisition and stimulation process.

limb movements. The EMG shield helps to customize the stimuli produced by the TENS device. The entire assembly used for acquisition and stimulation is depicted in figure 5.

**V. RESULTS AND DISCUSSION**

Experimentation is carried out in two phases, offline training phase and online recognition phase. Experimentation and validation are done on 10 healthy and 10 paralyzed subjects. In offline phase EEG activity of the paralyzed and EMG activity of the healthy subjects were recorded. In the training phase, subjects were given the familiarization of six different intended actions like, Grasp, Release, Rollup, Rolldown, Rollup Release etc. Multimedia feedback is given to the subjects to enhance the brain patterns. The subjects are enlightened by using encourages messages and appreciation speeches in the feedback, rather than simple live streaming the actions. Rollup-grasp, Rolldown-Release movements of the upper limb are used for communicating the need to the caregivers. In the online phase, user thoughts are recognized and converted into muscular action. The generated muscular action is correlated with the EMG activity of the healthy subjects. Based on the correlation result microcontroller selects the superior signal, which is used for stimulating the affected body part.

**A. RESULTS COMPARISON OF EEG ACTIVATED AND POSTURE ACTUATED MOVEMENTS**

Figure 6 shows the correlation of brain actuated real time EMG and posture actuated EMG for the subject intention to

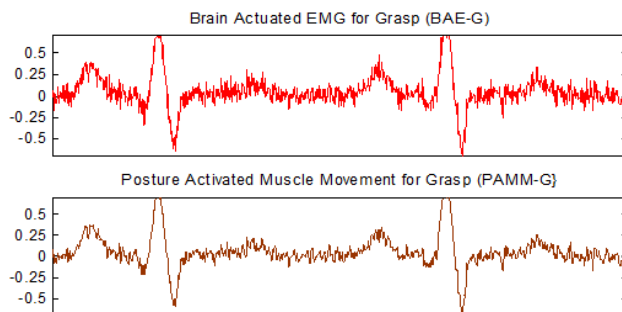


FIGURE 6. EMG activity for attempting grasp movements.

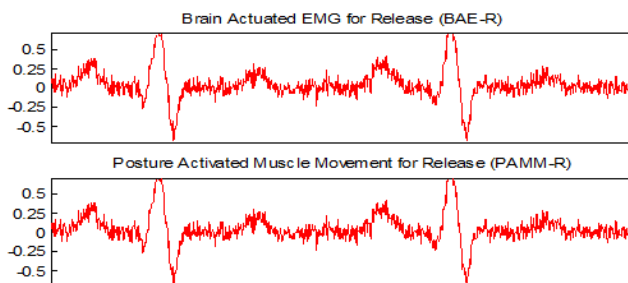


FIGURE 7. EMG variations corresponding to release movement.

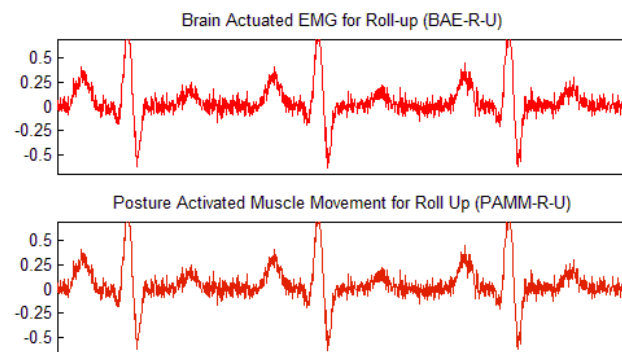


FIGURE 8. EMG activity based on ROLL up upper limb movement.

grasp the object. The EMG activity is recorded using EMG electrodes and measurement is done using Digital Storage Oscilloscope (DSO). The graph shows the amplitude variations of EMG signal with respect to frequency. The amplitude is normalized between  $\pm 0.5$ mv and frequency range used is 0-500Hz.

Figure 7 indicates the EMG variations observed in brain actuated and posture actuated movements corresponding to human intention of “Release”. Based on the correlation result brain actuated signal is selected for the stimulation of upper limb. Figure 8 shows the real time and recorded EMG activity for “Roll up” movement. Roll up movement is recorded using two electrodes placed on the either side of the Elbow. The rollup movement requires high intensity stimulation. In most of the time brain actuated EMG fallen below the desired level, so the stimulation of affected part is initiated in this case by artificial muscle movements. Figure 9 shows the EMG actuated by real time human Intention and the EMG activity produced using the training of “roll down” hand

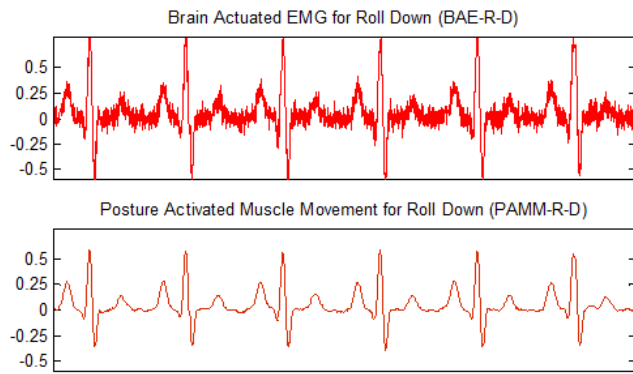


FIGURE 9. EMG activity based on ROLL down upper limb movement.


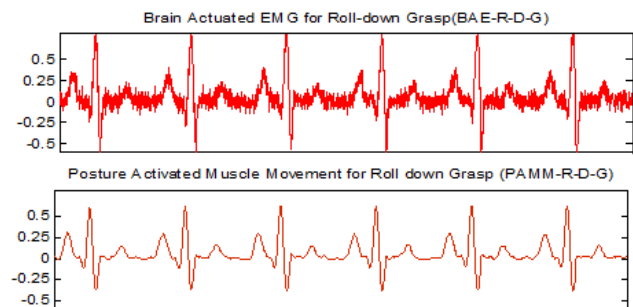


FIGURE 10. EMG activity for the gesture roll down-grasp.

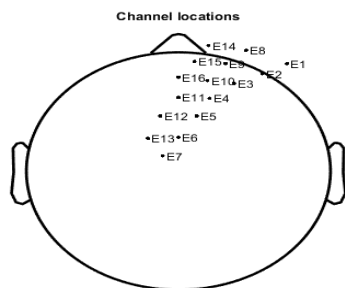

16 of 16 electrode locations shown

FIGURE 11. Electrode placement on the brain [21].

Posture. Roll down ideally requires low intensity signals, so in this movement selection priority is given to signal with low signal strength in the correlation. Figure 10 shows the EMG data acquired for the gesture “Roll down-grasp”. This EMG activity is used for communicating the paralyzed subject’s need to the caregivers.

**B. RESULT OF EEG PATTERNS ON THE REALISTIC HEAD MODELS**

Realistic head models are used for the analysis of EEG signals. EEG sensors with 16 electrodes are used for the capturing the brain signals. The unique electrode placement scheme used in this experimentation is shown in figure 11. The placement scheme mainly concentrated on the frontal and parietal regions of the brain.

The variations of brain patterns with different frequencies are analyzed to facilitate the feature extraction and classification process.

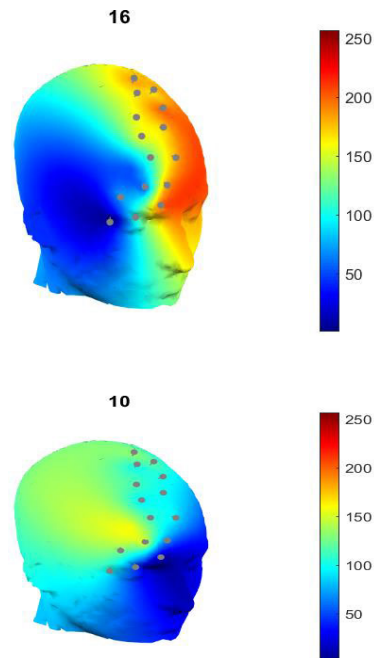


FIGURE 12. Brain pattern comparisons with and without multimedia feedback [21].

TABLE 2. Data statistics for brain actuated Rollup signal.

STATISTICAL PARAMETERS	X COEFFICIENT VALUES	Y COEFFICIENT VALUES
Min	1	0
Max	64	9
Mean	32.5	4.734
Median	32.5	5

In figure 12 red indicated the maximum interaction of neuron and blue indicates minimum interaction of neurons. The neuron connectivity in the head model on the left is improved when multimedia feedback is used, compared to the figure on right which does not use feedback.

**C. STATISTICAL ANALYSIS OF GENERATED EMG SIGNAL**

Statistical analysis is carried out to determine the correlation between Brain actuated EMG signal and posture actuated EMG signal. The data obtained during Rollup and Rolldown movement of the upper limb are utilized for the analysis.

Correlation matrix help to identify whether the human intentions match the recorded muscle movements. This matrix acts as a second level of classifier before the final actuation of the body part is made.

Correlation Matrix obtained  
[1.0000 0.0867 0.0867 1.0000]

Correlation matrix obtained  
[1.0000 -0.0640 -0.0640 1.0000]

Correlation matrix help to identify whether the human intentions match the recorded muscle movements.



**TABLE 3. Data statistics for posture actuated Rollup signal.**

Statistical parameters	X coefficient values	Y coefficient values
Min	1	-9.392
Max	64	8.982
Mean	32.5	-0.1296
Median	32.5	-0.09542
Mode	1	-9.392
Standard deviation	18.52	5.665

**TABLE 4. Data statistics for brain actuated Rolldown signal.**

Statistical parameters	X coefficient values	Y coefficient values
Min	1	0
Max	64	9
Mean	32.5	4.719
Median	32.5	4.5
Mode	1	0
Standard deviation	18.52	3.16


**TABLE 5. Data statistics for posture actuated Rollup signal.**

Statistical parameters	X coefficient values	Y coefficient values
Min	1	-9.392
Max	64	8.982
Mean	32.5	-0.1496
Median	32.5	-0.07542
Mode	1	-7.392
Standard deviation	18.52	4.665

This matrix acts as a second level of classifier before the final actuation of the body part is made.

**D. RESULTS OF CLASSIFICATION ACCURACY OF DIFFERENT SUBJECTS**

The classification accuracy of the system is verified by performing the test on 10 healthy subjects and 10 paralyzed persons. Maximum obtained 88% efficiency and on an average 80.45% classification accuracy based on the six different human intentions for upper limb movements. The experimentation result shown in figure 13 is the summary of results on 20 participants. U1-U10 are represent healthy subjects, U11-U20 represents paralyzed persons. The reason for improved accuracy for classification among subjects is

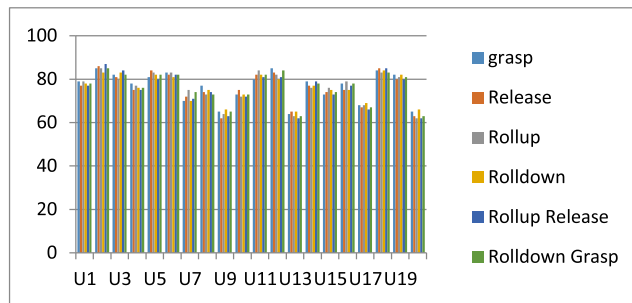

**FIGURE 13. Classification accuracy of six different movements on 20 subjects.**

due to systematic training undertaken and usage of feedback. The healthy subject U2 is an experienced user and is more familiar with similar interfaces, obtained high accuracy. However, the unhealthy subjects U11 and U12 also obtained high accuracy through their dedication and passion. Visual feedback and voice encouragement are also given to paralyzed during training. The participants U9 and U13 has shown similar low classification accuracy due to their age and unfamiliarity with the system

The authors used EEG signal to identify the human Intentions and to control upper limb movements of the paralyzed person. Artificial muscle movements are integrated into the system to get continuous movement of the affected body part. Recorded muscle movements help to enhance the rehabilitation process. The burden of carrying exoskeleton is avoided by incorporating by using innovative assembly. The communication aid for the paralyzed is provided by implementing gesture recognition module. AMIDL obtained better classification accuracy compared to many existing methods mentioned in the literature. The two-level classification employed in the system help to reduce false operations. The future research should focus on reducing human workload by incorporating efficient controllers. Accuracy of mapping human intentions with muscle movements has to be increased. Machine learning algorithms that can effectively map human intentions to the desired muscle movements are the way forward.

**VI. CONCLUSION**

AMIDL system with 3 different modular units is designed and implemented. The system validation is carried out by performing online and offline testing on 10 healthy and 10 paralyzed subjects. AMIDL is designed to perform six different movements like Grasp, Release, Rollup, Rolldown, Rollup Release, Rolldown Grasp on the paralyzed upper limb. WHT transform is utilized for feature extraction and classification of EEG signals. The EMG activity of the healthy subjects are correlated with the real-time EMG signals generated by the paralyzed. Selection criteria for the ideal signal is finalized based on the EMG analysis carried out on all six hand postures. The two-level classification method improved the accuracy of the system. The system produced continuous response even in the presence of uncertain real-time inputs.

Results indicate that mental fatigue and miss-operations are reduced. The burden of carrying exoskeleton is minimized by an innovative assembly having array of sensors and control units. Periodic stimulation in the absence of ideal brain signal enhance the rehabilitation process. Gesture Recognition method is utilized for providing communication aid for the paralyzed. In our future work, we are trying to incorporate closed loop controller with haptic feedback. Deep learning algorithms will be used to effectively map EEG signals with recorded EMG signals. The user experience can be enhanced by measuring the user emotions while performing the different activities.

## ACKNOWLEDGMENT

Authors would like to thank Ms. Asha Jacob, SCMS Center for Robotics for providing assistance and guidance in testing and conducting the experiments.

## REFERENCES

- [1] Christopher and Dana Reeve Foundation. *Paralysis statistics*. Accessed: Aug. 5, 2018. [Online]. Available: <https://www.christopherreeve.org/living-with-paralysis/stats-about-paralysis>
- [2] C. Watson, G. Paxinos, and G. Kayalioglu, Eds., *The Spinal Cord: A Christopher and Dana Reeve Foundation Text and Atlas*. New York, NY, USA: Academic, 2009.
- [3] P. Langhorne, J. Bernhardt, and G. Kwakkel, "Stroke rehabilitation," *Lancet*, vol. 377, no. 9778, pp. 1693–1702, 2011.
- [4] C. Wang, X. Wu, Z. Wang, and Y. Ma, "Implementation of a brain-computer interface on a lower-limb exoskeleton," *IEEE Access*, vol. 6, pp. 38524–38534, 2018.
- [5] J. M. Antelis, L. Montesano, A. Ramos-Murguialday, N. Birbaumer, and J. Minguez, "Decoding upper limb movement attempt from EEG measurements of the contralesional motor cortex in chronic stroke patients," *IEEE Trans. Biomed. Eng.*, vol. 64, no. 1, pp. 99–111, Jan. 2017.
- [6] E. Buch, C. Weber, L. G. Cohen, C. Braun, M. A. Dimyan, T. Ard, J. Mellinger, A. Caria, S. Soekadar, A. Fourkas, and N. Birbaumer, "Think to move: A neuromagnetic brain-computer interface (BCI) system for chronic stroke," *Stroke*, vol. 39, no. 3, pp. 910–917, 2008.
- [7] C. I. Penalzoa, M. Alimardani, and S. Nishio, "Android feedback-based training modulates sensorimotor rhythms during motor imagery," *IEEE Trans. Neural Syst. Rehabil. Eng.*, vol. 26, no. 3, pp. 666–674, Mar. 2018.
- [8] Y. Chae, J. Jeong, and S. Jo, "Toward brain-actuated humanoid robots: Asynchronous direct control using an EEG-based BCI," *IEEE Trans. Robot.*, vol. 28, no. 5, pp. 1131–1144, Oct. 2012.
- [9] Z. Li, W. Yuan, S. Zhao, Z. Yu, Y. Kang, and C. L. P. Chen, "Brain-actuated control of dual-arm robot manipulation with relative motion," *IEEE Trans. Cogn. Devel. Syst.*, vol. 11, no. 1, pp. 51–62, Mar. 2019.
- [10] T. D. Lalitharatne, K. Teramoto, Y. Hayashi, K. Tamura, and K. Kiguchi, "EEG-based evaluation for perception-assist in upper-limb power-assist exoskeletons," in *Proc. World Automat. Congr. (WAC)*, Aug. 2014, pp. 307–312.
- [11] I. Faiman, S. Pizzamiglio, and D. L. Turner, "Resting-state functional connectivity predicts the ability to adapt arm reaching in a robot-mediated force field," *NeuroImage*, vol. 174, pp. 494–503, Jul. 2018.
- [12] A. A. Frolov, O. Mokienko, R. Lyukmanov, E. Biryukova, S. Kotov, L. Turbina, G. Nadareyshivily, and Y. Bushkova, "Post-stroke rehabilitation training with a motor-imagery-based brain-computer interface (BCI)-controlled hand exoskeleton: A randomized controlled multicenter trial," *Frontiers Neurosci.*, vol. 11, p. 400, Jul. 2017.
- [13] N. A. Bhagat, A. Venkatakrishnan, B. Abibullaev, E. J. Artz, N. Yozbatiran, A. A. Blank, J. French, C. Karmonik, R. G. Grossman, M. K. O'Malley, J. L. Contreras-Vidal, and G. E. Francisco, "Design and optimization of an EEG-based brain machine interface (BMI) to an upper-limb exoskeleton for stroke survivors," *Frontiers Neurosci.*, vol. 10, p. 122, Mar. 2016.
- [14] H. A. Agashe, A. Y. Paek, and J. L. Contreras-Vidal, "Multisession, noninvasive closed-loop neuroprosthetic control of grasping by upper limb amputees," in *Progress in Brain Research*, vol. 228, 2016, ch. 4, pp. 107–128. doi: [10.1016/bs.pbr.2016.04.016](https://doi.org/10.1016/bs.pbr.2016.04.016).
- [15] J. Meng, S. Zhang, A. Bekyo, J. Olsoe, B. Baxter, and B. He, "Noninvasive electroencephalogram based control of a robotic arm for reach and grasp tasks," *Sci. Rep.*, vol. 6, Dec. 2016, Art. no. 38565.
- [16] F. Grimm, A. Walter, M. Spüler, G. Naros, W. Rosenstiel, and A. Gharabaghi, "Hybrid neuroprosthesis for the upper limb: Combining brain-controlled neuromuscular stimulation with a multi-joint arm exoskeleton," *Frontiers Neurosci.*, vol. 10, p. 367, Aug. 2016.
- [17] C. Vidaurre, C. Klauer, T. Schauer, A. Ramos-Murguialday, and K.-R. Müller, "EEG-based BCI for the linear control of an upper-limb neuroprosthesis," *Med. Eng. Phys.*, vol. 38, no. 11, pp. 1195–1204, Nov. 2016.
- [18] Z. Tang, S. Sun, S. Zhang, Y. Chen, C. Li, and S. Chen, "A brain-machine interface based on ERD/ERS for an upper-limb exoskeleton control," *Sensors*, vol. 16, no. 12, p. 2050, 2016.
- [19] B. Xu, A. Song, G. Zhao, G. Xu, L. Pan, R. Yang, H. Li, and J. Cui, "Design and evaluation of a motor imagery electroencephalogram-controlled robot system," *Adv. Mech. Eng.*, vol. 7, no. 3, 2015, Art. no. 1687814015573607.
- [20] A. M. Elnady, X. Zhang, Z. G. Xiao, X. Yong, B. K. Randhawa, L. Boyd, and C. Menon, "A single-session preliminary evaluation of an affordable BCI-controlled arm exoskeleton and motor-proprioception platform," *Frontiers Hum. Neurosci.*, vol. 9, p. 168, Mar. 2015.
- [21] V. P. G. S. Jacob, V. G. Menon, S. Rajesh, and M. R. Khosravi, "Brain-controlled adaptive lower limb exoskeleton for rehabilitation of post-stroke paralyzed," *IEEE Access*, to be published.
- [22] S. Jacob, "A review of technology advances for assisting paralyzed people [leading edge]," *IEEE Technol. Soc. Mag.*, vol. 36, no. 2, pp. 36–37, Jun. 2017.
- [23] S. Rajesh, V. Paul, V. G. Menon, and M. R. Khosravi, "A secure and efficient lightweight symmetric encryption scheme for transfer of text files between embedded IoT devices," *Symmetry*, vol. 11, no. 2, p. 293, 2019.
- [24] P. G. Vinoj, S. Jacob, and V. G. Menon, "Hybrid brainactuated muscle interface for the physically disabled," *Basic Clin. Pharmacol. Toxicol.*, vol. 123, pp. 8–9, Sep. 2018.
- [25] M. Al-Quraishi, I. Elamvazuthi, S. Daud, S. Parasuraman, and A. Borboni, "EEG-based control for upper and lower limb exoskeletons and prostheses: A systematic review," *Sensors*, vol. 18, no. 10, p. 3342, Oct. 2018.
- [26] D. Brauchle, M. Vukelić, R. Bauer, and A. Gharabaghi, "Brain state-dependent robotic reaching movement with a multi-joint arm exoskeleton: Combining brain-machine interfacing and robotic rehabilitation," *Frontiers Hum. Neurosci.*, vol. 9, p. 564, Oct. 2015.
- [27] S. Comani, L. Velluto, L. Schinaia, G. Cerroni, A. Serio, S. Buzzelli, B. Guarnieri, and S. Sorbi, "Monitoring neuro-motor recovery from stroke with high-resolution EEG, robotics and virtual reality: A proof of concept," *IEEE Trans. Neural Syst. Rehabil. Eng.*, vol. 23, no. 6, pp. 1106–1116, Nov. 2015.
- [28] F. Grimm, A. Walter, M. Spüler, G. Naros, W. Rosenstiel, and A. Gharabaghi, "Hybrid neuroprosthesis for the upper limb: Combining brain-controlled neuromuscular stimulation with a multi-joint arm exoskeleton," *Frontiers Neurosci.*, vol. 10, p. 367, Aug. 2016.
- [29] S. R. Soekadar, M. Witkowski, N. Vitiello, and N. Birbaumer, "An EEG/EOG-based hybrid brain-neural computer interaction (BNCI) system to control an exoskeleton for the paralyzed hand," *Biomed. Eng./Biomedizinische Technik*, vol. 60, no. 3, pp. 199–205, 2015.
- [30] E. A. Kirchner, M. Tabie, and A. Seeland, "Multimodal movement prediction—Towards an individual assistance of patients," *PLoS ONE*, vol. 9, no. 1, 2014, Art. no. e85060.
- [31] R. Looned, J. Webb, Z. G. Xiao, and C. Menon, "Assisting drinking with an affordable BCI-controlled wearable robot and electrical stimulation: A preliminary investigation," *J. Neuroeng. Rehabil.*, vol. 11, no. 1, p. 51, 2014.
- [32] M. Steinisch, M. G. Tana, and S. Comani, "A post-stroke rehabilitation system integrating robotics, VR and high-resolution EEG imaging," *IEEE Trans. Neural Syst. Rehabil. Eng.*, vol. 21, no. 5, pp. 849–859, Sep. 2013.
- [33] S. W. Tung, C. Guan, K. K. Ang, K. S. Phua, C. Wang, L. Zhao, W. P. Teo, and E. Chew, "Motor imagery BCI for upper limb stroke rehabilitation: An evaluation of the EEG recordings using coherence analysis," in *Proc. 35th Annu. Int. Conf. IEEE Eng. Med. Biol. Soc. (EMBC)*, Jul. 2013, pp. 261–264.
- [34] A. Ramos-Murguialday, M. Schürholz, V. Caggiano, M. Wildgruber, A. Caria, E. M. Hammer, S. Halder, and N. Birbaumer, "Proprioceptive feedback and brain computer interface (BCI) based neuroprostheses," *PLoS ONE*, vol. 7, no. 10, 2012, Art. no. e47048.

- [35] A. Frisoli, C. Loconsole, D. Leonardi, F. Banno, C. Chisari, M. Bergamasco, and M. Barsotti, "A New Gaze-BCI-Driven Control of an Upper Limb Exoskeleton for Rehabilitation in Real-World Tasks," *IEEE Trans. Syst., Man, Cybern. C, Appl. Rev.*, vol. 42, no. 6, pp. 1169–1179, Nov. 2012.
- [36] F. Al-Turjman, H. Zahmatkesh, and R. Shahroze, "An overview of security and privacy in smart cities' IoT communications," *Trans. Emerg. Telecommun. Technol.*, Jul. 2019, Art. no. e3677. doi: 10.1002/ett.3677.
- [37] S. Kutia, S. H. Chauhdary, C. Iwendu, L. Liu, W. Yong, and A. K. Bashir, "Socio-Technological factors affecting user's adoption of eHealth functionalities: A case study of China and Ukraine eHealth systems," *IEEE Access*, vol. 7, pp. 90777–90788, 2019.
- [38] F. Al-Turjman and I. Baali, "Machine learning for wearable IoT-based applications: A survey," *Trans. Emerg. Telecommun. Technol.*, May 2019, Art. no. e3635. doi: 10.1002/ett.3635.
- [39] V. Anavangot, V. G. Menon, and A. Nayyar, "Distributed big data analytics in the Internet of signals," in *Proc. Int. Conf. Syst. Modeling Advancement Res. Trends (SMART)*, Nov. 2018, pp. 73–77.
- [40] D. K. Jain, S. Jacob, V. Menon, and J. Alzubi, "An efficient and adaptable multimedia system for converting PAL to VGA in real-time video processing," *J. Real-Time Image Process.*, pp. 1–13, Jun. 2019. doi: 10.1007/s11554-019-00889-4.
- [41] F. Al-Turjman, H. Zahmatkesh, and L. Mostarda, "Quantifying uncertainty in Internet of medical things and big-data services using intelligence and deep learning," *IEEE Access*, vol. 7, pp. 115749–115759, 2019.
- [42] F. Al-Turjman, "Intelligence and security in big 5G-oriented IoT: An overview," *Future Gener. Comput. Syst.*, vol. 102, pp. 357–368, Jan. 2020.
- [43] L. Feng, A. Ali, M. Iqbal, A. K. Bashir, S. A. Hussain, and S. Pack, "Optimal haptic communications over nanonetworks for E-health systems," *IEEE Trans. Ind. Informat.*, vol. 15, no. 5, pp. 3016–3027, 2019.
- [44] B. Xu, S. Peng, A. Song, R. Yang, and L. Pan, "Robot-aided upper-limb rehabilitation based on motor imagery EEG," *Int. J. Adv. Robotic Syst.*, vol. 8, no. 4, p. 40, 2011.
- [45] H. K. Yap, N. Kamaldin, J. H. Lim, F. A. Nasrallah, J. C. H. Goh, and C.-H. Yeow, "A magnetic resonance compatible soft wearable robotic glove for hand rehabilitation and brain imaging," *IEEE Trans. Neural Syst. Rehabil. Eng.*, vol. 25, no. 6, pp. 782–793, Jun. 2017.
- [46] H. S. Nam, S. Koh, Y. J. Kim, J. Beom, W. H. Lee, S.-U. Lee, and S. Kim, "Biomechanical reactions of exoskeleton neurorehabilitation robots in spastic elbows and wrists," *IEEE Trans. Neural Syst. Rehabil. Eng.*, vol. 25, no. 11, pp. 2196–2203, Nov. 2017.



**SUNIL JACOB** is currently the Director with the Centre for Robotics, SCMS School of Engineering and Technology, and also a Professor with the Department of Electronics and Communication Engineering. He was a recipient of the AICTE ChathraVishvakarma Award, in electronics, in 2017, and the Young Gandhian Technological Innovation Appreciation Award, in 2018. His project Muscles to Machine Interface for Paralyzed has been funded by IEEE EPICS USA, and other funded projects include bionic haptic arm, rejuvenating the cells of human body, de-addiction coil for drug addicts, smart keyboard for disabled person, low cost 3D printer, and wearable device for detection and prevention of heart failure.



**VARUN G. MENON** is currently an Associate Professor with the Department of Computer Science and Engineering, SCMS School of Engineering and Technology and the Head of International Partnerships with the SCMS Group of Educational Institutions, India. His current research interests include the Internet of Things, brain-computer interface, mobile ad-hoc networks, wireless communication, opportunistic routing, wireless sensor networks, fog computing and networking, and underwater acoustic sensor networks. He is also Distinguished Speaker with the Association of Computing Machinery (ACM). He is currently serving as a Guest Editor of the *Journal of Supercomputing*. He is currently serving on the Review Boards of the IEEE TRANSACTIONS ON VEHICULAR TECHNOLOGY, the IEEE TRANSACTIONS ON COMMUNICATIONS, and the *IEEE Communications Magazine*.



**FADI AL-TURJMAN** (M'07) received the Ph.D. degree in computer science from Queen's University, Canada, in 2011. He is currently a Professor with Antalya Bilim University, Turkey. He is also a leading authority in smart/cognitive, wireless and mobile networks' architectures, protocols, deployments, and performance evaluation. His record spans more than 200 publications in journals, conferences, patents, books, and book chapters, in addition to numerous keynotes and plenary talks at flagship venues. He has authored or edited more than 12 published books about cognition, security, and wireless sensor networks' deployments in smart environments with Taylor & Francis and Springer (Top tier publishers in the area). He was a recipient of several recognitions and best papers' awards at top international conferences. He also received the prestigious Best Research Paper Award from Elsevier COMCOM Journal for the last three years, prior to 2018, in addition to the Top Researcher Award for 2018 at Antalya Bilim University, Turkey. He led a number of international symposia and workshops in flag-ship IEEE ComSoc conferences. He is serving as the Lead Guest Editor in several journals, including the *IET Wireless Sensor Systems*, Springer, EURASIP, *MDPI Sensors*, Wiley&Hindawi WCM, and the Elsevier COMCOM and *Internet of Things*.



**VINOJ P. G.** received the B.Tech. degree in electronics and communication from the Cochin University of Science and Technology, Cochin, India, in 2004, and the M.Tech. degree in embedded system from the National Institute of Electronics and Information Technology, Calicut, India, in 2008. He is currently pursuing the Ph.D. degree in electronics and communication engineering with APJ Abdul Kalam Technological University, Kerala, India. He was a Researcher with Robhatah Robotic Solution, Bangalore. He is currently an Assistant Professor with the Department of Electronics and Communication, SCMS School of Engineering and Technology and an Associate Member of the Center for Robotics.



**LEONARDO MOSTARDA** received the Ph.D. degree from the Computer Science Department, University of L'Aquila, in 2006. He cooperated with the European Space Agency (ESA) on the CUSPIS FP6 Project to design and implement novel security protocols and secure geo tags for works of art authentication. To this end, he was combining traditional security mechanisms and satellite data. In 2007, he was a Research Associate with the Distributed System and Policy Group, Computing Department, Imperial College London, where he was involved in the UBIVAL EPRC Project in cooperation with Cambridge, Oxford, Birmingham, and UCL for building a novel middleware to support the programming of body sensor networks. In 2010, he was a Senior Lecturer with the Distributed Systems and Networking Department, Middlesex University, where he founded the Senso LAB, an innovative research laboratory for building energy efficient wireless sensor networks. He is currently an Associate Professor and the Head of Computer Science Department, University of Camerino, Italy.

...