

# Using a Sniff Controller to Self-Trigger Abdominal Functional Electrical Stimulation for Assisted Coughing Following Cervical Spinal Cord Lesions

Lior Haviv, Hagit Friedman, Uri Bierman, Itzhak Glass, Anton Plotkin, Aharon Weissbrod, Sagit Shushan, Vadim Bluvshstein, Elena Aidinoff, Noam Sobel, and Amiram Catz

**Abstract**—Individuals with cervical spinal cord lesions (SCLs) typically depend on caregivers to manually assist in coughing by pressing against their abdominal wall. Coughing can also be assisted by functional electrical stimulation (FES) applied to abdominal muscles via surface electrodes. Efficacy of FES, however, depends on precise temporal synchronization. The sniff controller is a trigger that enables paralyzed individuals to precisely control external devices through alterations in nasal airflow. We hypothesized that FES self-triggering by sniff controller may allow for effective cough timing. After optimizing parameters in 16 able-bodied subjects, we measured peak expiratory flow (PEF) in 14 subjects with SCL who coughed with or without assistance. Assistance was either manual assistance of a caregiver, caregiver activated FES, button self-activated FES (for SCL participants who could press a button), or sniff-controlled self-activated FES. We found that all assisted methods provided equally effective improvements, increasing PEF on average by  $25 \pm 27\%$  ( $F[4, 52] = 7.99, p = 0.00004$ ). There was no difference in efficacy between methods of assistance ( $F[3, 39] = 0.41, p = 0.75$ ). Notably, sniff-controlled FES was the only method of those tested that can be activated by all paralyzed patients alone. This provides for added independence that is a critical factor in quality of life following SCL.

**Index Terms**—Assistive technology, cough, functional electrical stimulation (FES), sniff-controller, spinal cord lesion (SCL).

Manuscript received April 6, 2016; revised September 5, 2016; accepted October 24, 2016. Date of publication January 31, 2017; date of current version September 2, 2017. This study was supported by grant P-144 to Professor Noam Sobel from IRP – International Foundation for Research in Paraplegia.

L. Haviv, A. Plotkin, A. Weissbrod, S. Shushan, and N. Sobel are with the Department of Neurobiology, Weizmann Institute of Science, Rehovot 76100, Israel (e-mail: liorhaviv100@gmail.com; plotkin.anton@gmail.com; aharon.weissbrod@weizmann.ac.il; sashushan@gmail.com; noam.sobel@weizmann.ac.il).

H. Friedman is with the Department of Nursing, Faculty of Social Welfare and Health Sciences, University of Haifa, Haifa 3498838, Israel (e-mail: hmts@netvision.net.il).

U. Bierman, and I. Glass are with Loewenstein Rehabilitation Hospital, Ra'anana 43100, Israel.

V. Bluvshstein, E. Aidinoff, and A. Catz are with Loewenstein Rehabilitation Hospital, Ra'anana 43100, Israel, and also with the Sackler Faculty of Medicine, Tel-Aviv University, Tel-Aviv 6997801, Israel (e-mail: vadimb3@clalit.org.il; aidinofe@clalit.org.il; amiramc@clalit.org.il).

Digital Object Identifier 10.1109/TNSRE.2016.2632754

## I. INTRODUCTION

THERE are between 250,000 and 500,000 new cases of spinal cord lesions (SCLs) worldwide annually. SCLs are associated with an elevated risk of death, mostly during the first year after lesion [1]. Different secondary conditions, such as pneumonia, pressure ulcers and urinary tract infections are a major cause of morbidity and mortality following SCL [2], [3]. These conditions frequently lead to hospitalization and can also result in increased costs of care, reduced employability, decreased quality of life and lowered life expectancy [1], [2], [4]–[6]. Respiratory complications, which are among the major causes of morbidity and mortality after SCL, may occur in patients with lower cervical or high thoracic SCL. These complications occur in part because of paralysis of the abdominal muscles, which are required for expiration in the upright position, support effective inspiration [7], [8] and enable coughing. Coughing is necessary for efficient removal of secretions and solid particles from the respiratory tracts [9]. Impairment of coughing may cause bronchial obstruction and consequent atelectasis pneumonia with severe respiratory disturbances [7]. Therefore, when abdominal muscles are paralyzed, external assistance is required for coughing. At present, an individual with SCL who needs assistance for coughing frequently depends on a caregiver applying intermittent manual pressure to the anterior abdominal wall [10], [11].

To minimize dependency on a caregiver, individuals with SCL frequently use assistive technologies. They may need assistive technology just after injury, or throughout life. The level of the SCL and associated impairments, environmental factors, personal factors and comorbid health conditions influence the type of required assistive technology. Assistive technologies can include mobility devices, communication devices, aids for self-care, and aids for domestic activities and environmental control systems that help in daily function [1]. In the case of coughing, there are several available assistive technologies: These include manual air stacking, or glossopharyngeal breathing (GPB), where the patient basically gulps boluses of air to later be expired as a cough. These gulps of air can be self-generated or manually assisted [12], [13]. Air stacking depends on an intact glottis, and if this fails an

added one-way flow valve type device can compensate for air leakage [14]. Additionally, small manual devices that combine high-frequency airflow oscillations with positive expiratory pressure (PEP) can be used to assist in coughing [15]. In turn, several approaches can be used to externally activate abdominal muscles, one of which is functional electric stimulation (FES) applied to abdominal muscles [8], [16]–[21]. This method, however, is not always effective, possibly due to the lack of synchronization accuracy in FES triggering. In coughing, afferent impulses of the cough reflex processed by the brain-stem cause a series of synchronized events in the following order: (I) air inspiration; (II) tight closure of the glottis and vocal cords to trap the air within the lungs; (III) forceful contraction of abdominal muscles and accessory expiratory muscles to increase air pressure within the lungs; and (IV) sudden opening of the vocal cords to enable the immediate forceful blowing out of air with secretions and solid particles [22]. This series of events requires precise synchronization in order to evoke an effective cough, and the timing of its activation by FES is critical for the synchronization between glottis closure and abdominal muscle contraction.

Several previous studies reported FES triggering using physiological measures. These included electromyographic (EMG) signals from either the pectoralis major muscle or the deltoid muscle [20], as well as various measures of respiration [23]–[28] (more on this in the discussion). Here we set out to investigate a novel alternative for FES control, namely the sniff-controller. The sniff-controller detects slight perturbations in nasal airflow and converts these into electrical signals that can control external devices [29]. Because nasal airflow is modulated in part by the soft palate [30], which is innervated by cranial nerves [31], [32], the sniff-controller remains functional following any type of SCL [29]. The sniff-controller can be programmed to control a host of assistive technologies ranging from mobility to communication. Its application to FES triggering may be particularly appropriate because sniff-controller activation and cough mechanisms likely rely on common neural substrates of respiration. For example, c-Fos studies in cats have identified several brainstem structures involved in both sniff and cough [33], [34]. These include the nuclei of the solitary tract, the lateral reticular nucleus, the medullary raphe nuclei, and the parabrachial and Kölliker-Fuse nuclei of the pons [33], [34]. Moreover, several lines of evidence imply a critical role for the Böttinger complex in both sniffing [35] and coughing [36]. With this in mind, we set out to optimize FES triggering by sniff-controller in able-bodied subjects, and then applied this optimized system in individuals with SCL, where we compared its performance to non-assisted and assisted coughing.

## II. METHODS

### A. Subjects

We approached current and past patients of the Loewenstein rehabilitation hospital. Inclusion criteria were: Tetraplegic men and women aged 20 to 60 years, with complete low cervical or high thoracic SCL (ASIA grade A or B) with motor impairment related to segments C4–T6. Exclusion criteria were: Respiratory difficulties not directly related to the

**TABLE I**  
FOURTEEN PARTICIPANTS WITH SCL, DETAILING LEVEL OF SPINAL INJURY, ASIA GRADE, TIME FROM IN YEARS, GENDER AND AGE

Subject	Injury Level	ASIA Grade	Time From Injury (Years)	Gender	Age
1	C6	C	3	M	35
2	T2	A	15	M	42
3	C4	A	10	M	56
4	T4	A	6	M	33
5	T4	A	5	M	47
6	C5	A	7	M	37
7	T4	A	3	M	41
8	T4	A	37	M	57
9	C4	A	11	M	48
10	C6	A	8	M	35
11	C5	B	17	M	50
12	C5	A	9	F	21
13	C6	A	2	M	24
14	C5	B	10	F	29


spinal injury; Pacemaker; Electronic implant; Pressure wound; Pregnancy; Inability to communicate with the experimenter. For able-bodied participants we applied the same exclusion criteria. These criteria yielded 16 able-bodied subjects (4 women, age: 25-44 years) and 14 subjects with low cervical or high thoracic SCL (2 women, age: 21-57 years) who all participated in the study after providing informed consent to procedures approved by the Helsinki Committee of Loewenstein Rehabilitation Hospital. Notably, some of the patients had sporadically experienced FES long before this study, but none of them were regular users. Additional details on participants with SCL are available in Table I.

### B. Characterizing Nasal Airflow During Cough Events

Our aim was to mimic the natural cough reflex. This includes precise synchronization of abdominal muscle contraction and progressive glottis closure. We therefore conducted experiments designed to characterize the temporal relation of these events with nasal airflow and muscle activity in the anterior neck and abdomen. To this end we developed an experimental setup that included an endoscopic video camera (Portable Bedside Laryngoscope, Distal Tip 3.4 mm, PENTAX) that was synchronized with nasal airflow measurement, a microphone, and a signal amplifier (ETH-256, iWorx Systems, Inc.) for EMG of the anterior neck and abdominal muscles as illustrated in Fig. 1. For measuring airflow we used a nasal cannula linked to a sniff controller device [29]. Data was recorded using an instrumentation amplifier (ADInstruments PowerLab 8SP) at 1 kHz and LabChart 7 for Mac software (ADInstruments). Note that this setup with video camera and EMG was applied in the able-bodied subjects only.

### C. Integration of the Sniff Controller With FES

The system used for computerized control of the FES incorporated the sniff controller technology that included an Arduino microcontroller device (www.arduino.org). The microcontroller received analog inputs from the airflow sensors and was programmed to trigger the FES. This system

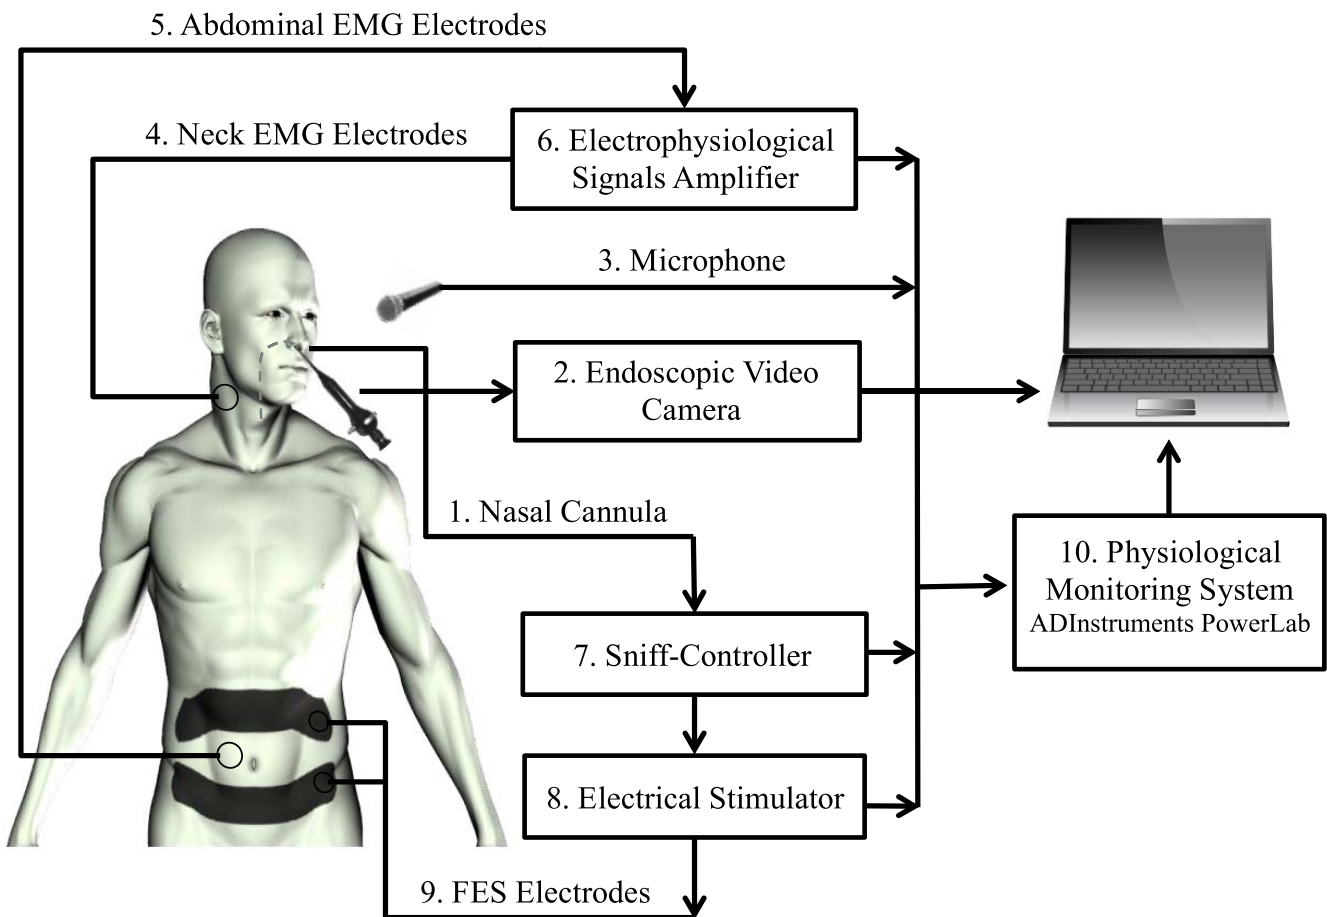

**Fig. 1.** The experimental apparatus used in able-bodied participants. We obtained simultaneous measurements during coughing from: 1. Nasal cannula, 2. Endoscopic video camera, 3. Microphone, 4. Neck EMG, 5. Abdominal EMG, 6. Electrophysiological Signals Amplifier, 7. Sniff-Controller, 8. Electrical stimulator, 9. FES electrodes. We placed electrodes in two rows. Each row contained four electrodes connected to a single pole of the stimulator. This made for effectively two large stimulating electrodes as illustrated. 10. Physiological monitoring system (ADInstruments Powerlab).

can switch between manual and self-activation modes using a standby button. The standby status can be set in place using a sniff-controller command. After defining the features of the nasal respiration pattern that indicate the progressive glottis closure, we developed software that continuously samples the sniff trace and detects the defined features. This software is here made publically available in the Supplementary Materials (note that instructions for construction of a complete sniff-controller have also been made publically available at <http://www.snifflogic.org/#!diy> such that the entire device described in this manuscript can be constructed with relative ease).

#### D. FES Experimental Setup

Stimulation was delivered by Constant Current Stimulator (DS7A, Digitimer), using self-adhesive surface electrodes [Size 5 cm x 13 cm, Model 895250, AXELGAARD) directly over the abdominal muscles of SCL subjects lying in the supine position. A constant current of 240 mA (0.92 mA/cm<sup>2</sup>) was delivered for 500 ms, which consisted a train of 200  $\mu$ s monophasic square pulses at 100 Hz. Given that the effectiveness of FES increases with stimulus intensity and plateaus at  $\sim$ 211 mA [37], our selection of 240 mA puts us well within

this optimal range. FES is often applied bilaterally using four separate electrode pairs [23]. In the present study we used a different configuration of stimulating electrodes (Fig. 1): Four self-adhesive surface electrodes were situated in a row next to each other on the abdominal muscles above the umbilicus, and were connected in parallel to one output pole of the stimulator. Similarly, another set of four electrodes was situated under the umbilicus, and was connected the other output pole. This effectively constituted two large stimulating electrodes (260 cm<sup>2</sup> each) aimed at maximizing the stimulated area.

#### E. Cough Efficacy Experiments

We tested cough efficacy comparing five different methods for cough induction: 1. Without assistance. 2. With manually assisted expiration (by a physiotherapist). 3. FES-assisted expiration activated by a caregiver. 4. Button-press self activated FES-assisted expiration. 5. Sniff-Controller-FES automatic activation. To assess the effects of the different methods for increasing the intra-abdominal pressure during cough and breathing we measured peak expiratory flow (PEF) during cough. In other words, PEF was the measure of cough efficacy in this study. We also measured forced vital capacity (FVC),

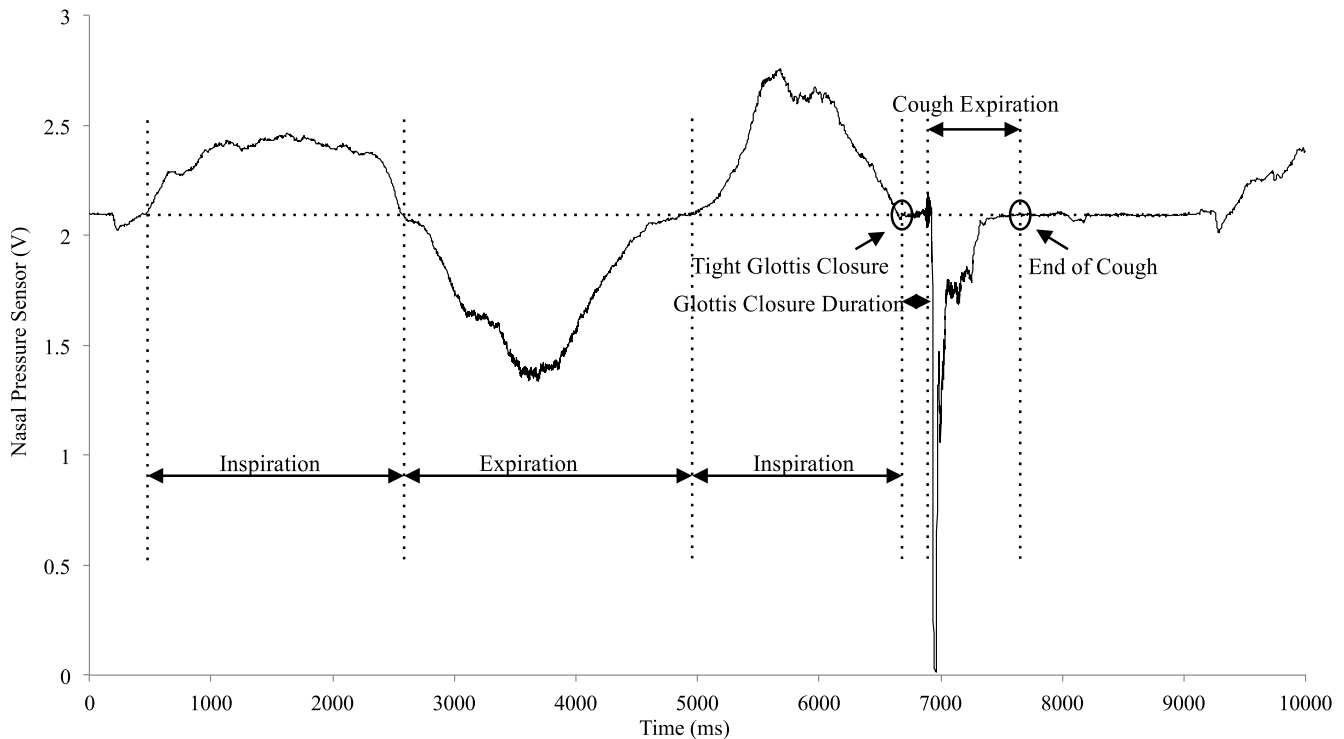


Fig. 2. Nasal respiratory pattern during progressive cough events in an able-bodied subject. The ordinate is signal from the sniff-controller reflecting nasal airflow (converted into volts). The dotted horizontal line reflects baseline, or the point of shift between inhalation and exhalation. Individual events such as glottis closure were obtained through simultaneous endoscopic video

and maximal voluntary ventilation (MVV) after cough. Lung functions after cough were measured in the supine position and with nostrils sealed by nasal clips, using a Pony FX device and Omnia 1.2 (COSMED, Italy) software. The participants were encouraged to achieve maximal capacity in the respiratory tests, and the best of three attempts was included in the analysis. The order of tests was sequenced randomly.

#### F. Statistical Analyses

The modes of cough (assistance and its types) were submitted to a within-subjects repeated-measures analyses of variance (ANOVA) followed by planned comparisons with t-tests for each variable (PEF, FVC, MVV). Data were analyzed using STATISTICA for Windows (version 7.0; StatSoft, Inc., Tulsa, OK, USA). The use of within-subjects tests minimized any impact of individual differences in extent of injury and impairment.

### III. RESULTS


#### A. Identifying the Sniff-Controller Time Point for FES Activation

To characterize the pattern of nasal respiration during cough we first tested eight able-bodied subjects who were asked to breathe through their nose and cough spontaneously. We recorded the progressive events that involve coughing, as shown in Fig. 2. Respiration airflow rates higher and lower than baseline correspond to inspiration and expiration, respectively. The cough sequence is characterized by higher


peak flow compared to the prior inhalation (Fig. 2), which is the first event of the cough process. The second event is tight closure of the glottis to trap air within the lungs. The initiation of glottis closure is associated with a rapid decrease of the inspiration flow rate towards zero or baseline, followed by a relatively small local peak of expiration flow rate (as marked by left circle in Fig. 2). This peak, observed in 98% of cases, can be related to measured pressure vibrations resulting from the rapid complete closure of the glottis. Examination of the endoscopic video synchronized with nasal airflow measurement suggested that glottis closure begins with vocal cord shutting followed by progressive contraction of the glottis spanning several milliseconds. The mean time difference between the visualized glottis closure and the following local minimum of respiration flow rate was  $45 \pm 40$  ms (Fig. 3 and Online Video). During the third event, which is a spontaneous forceful contraction of abdominal muscles and accessory expiratory muscles, the glottis remained closed. Thus, airflow is halted and as expected, we observed a plateau of the respiration flow rate, until opening of the glottis. We found that the mean glottis closure duration was  $411 \pm 218$  ms. The last event in the cough process, a sudden opening of the glottis and vocal cords and outward expulsion of the air under pressure, is clearly evidenced in the sniff trace.

The above parameters were identified during normal breathing that is predominantly nasal. To estimate the value of the residual nasal signal evident during oral breathing we again tested the system in eight able-bodied subjects who were asked to breathe through the mouth and cough voluntarily.



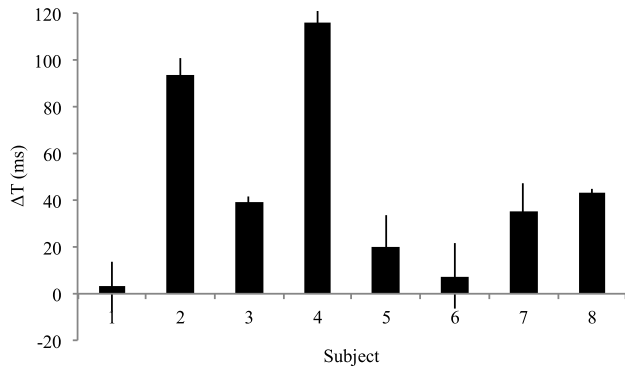


**Fig. 3.** Time difference ( $\Delta T$ ) between glottis closure and respiration minima. The ordinate is time difference in milliseconds and the abscissa is subject serial number. Bars are SE.

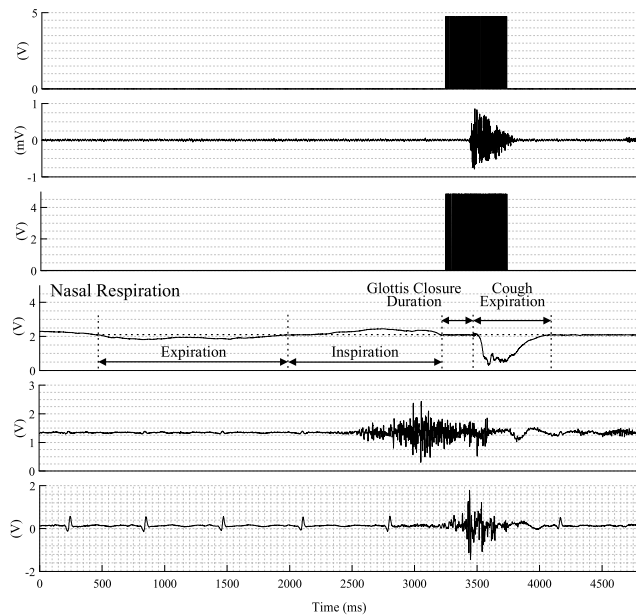

**Fig. 4.** Timeline of experimental events. Experimental measurements of nasal respiratory pattern synchronized with sound recording and EMG of neck and abdominal muscles in an able-bodied subject.

We observed that nasal respiration was idiosyncratic for each individual and the dynamics of the soft palate were changed during the experiment. This was reflected by differentiation of the inhalation peak, the negative slope rate, the local minimum of the flow rate and glottis closure duration. Nevertheless, the sniff-controller continuously measured airflow during cough, detected the timing of glottis closure (the local minimum of the flow rate of respiration) and emitted a FES-activation signal with a pre-defined delay (50 ms) (Fig. 4) (note that FES stimulation was not delivered to the able-bodied subjects). In other words, the system synchronized cough detection and FES activation at the time frame of natural coughing even when respiration was not intentionally nasal. As cough was detected, the sniff-controlled device activated the stimulator to elicit a pulse train at a frequency of 100 Hz for 500 ms, with a pre-determined delay after the minimum time-point. The system response was highly accurate; the mean delayed time of FES triggering was  $36 \pm 8$  ms, which was immediately followed by stimulator output (Fig. 4). The mean

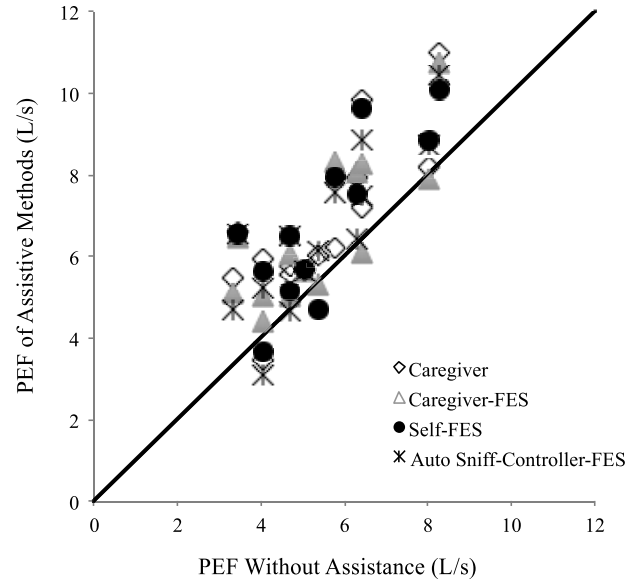

**Fig. 5.** Assisted coughing improves cough. All methods compared along the unit slope-line. Each dot is a subject at a method as indicated by the color and style legend. All assisted methods were better than unassisted (all dots above the line), and there was no difference between assistive methods.

duration of the glottis closure was  $411 \pm 218$  ms in subjects that were asked to breath regularly (mostly nasaly), and cough voluntarily, but only  $187 \pm 83$  ms in those who were asked to breath through the mouth and cough. Inhalation was deeper before cough in 91% of the cases, higher than the previous inhalation by  $10 \pm 5\%$ .

### B. Activity of Neck and Abdominal Muscles During Cough

We recorded EMG signals from abdominal and neck muscles during cough in eight able-bodied subjects. We found that the abdominal muscle contraction was a progressive process that on average remained active for  $559 \pm 310$  ms. Activity started  $174 \pm 275$  ms before glottis closure, and in 30% of the cases it was also observed after glottis closure (Fig. 4). Furthermore, neck muscle activity started before abdominal muscle activity, and  $415 \pm 240$  ms before the onset of minimal airflow, and in total lasted together with glottis muscle activity for  $826 \pm 347$  ms.

### C. Cough Efficacy of Assistive Methods

Fourteen subjects with SCL participated in this part of the study. Once the sniff-controller was put in stand-by mode (this can be done by a key-board command or by a sniff-controller command, e.g., sniff in-out-in within one second), it triggered FES activation based on the above results. Specifically, given the above-observed difference of  $45 \pm 40$  ms between the airflow minima and full glottis closure, the trigger was activated 50 ms after airflow minima. We then individually fine-tuned the delay, based on patient self-report of cough efficacy during 3-5 test-coughs. This resulted in an average delay of  $152 \pm 70$  ms, which is  $67\% \pm 20\%$  of the glottis closure

**TABLE II**  
COUGH EFFICACY OF ASSISTIVE METHODS

Subject	PEF [L/s]	PEF Ratio Assistive/Unassistive	Time Ratio Trigger Onset/Glottis Closure Duration
No assistance	5.42 ± 1.55	-	-
Caregiver	6.77 ± 1.93	1.28 ± 0.28	-
Caregiver-FES	6.60 ± 1.79	1.25 ± 0.25	0.33 ± 0.53
Manually Self-FES	6.83 ± 2.01	1.26 ± 0.28	0.78 ± 0.26
Auto Sniff Controller-FES	6.57 ± 1.94	1.23 ± 0.27	0.67 ± 0.20

The five methods of coughing tested in this study, and the associated PEF values with each (mean ± SD), as well as the factor of improvement over unassisted coughing.

duration (The delay time was normalized according to glottis closure duration for each subject). Three subjects retained the unoptimized 50 ms window. An ANOVA on PEF values during cough with conditions of assistance (assisted/unassisted) and mode (caregiver/caregiver-FES/self-FES/sniff controller) revealed a main effect of assistance ( $F[4, 52] = 7.99$ ,  $p = 0.00004$ ), and no effect of mode ( $F[3, 39] = 0.41$ ,  $p = 0.75$ ). Planned comparisons revealed that this reflected a significant increase in PEF with assistance, but no difference between assistive methods (mean PEF unassisted =  $5.42 \pm 1.55$  L/s, mean PEF caregiver =  $6.77 \pm 1.93$  L/s, mean PEF caregiver-FES =  $6.60 \pm 1.79$  L/s, mean PEF self-FES =  $6.83 \pm 2.01$  L/s, mean PEF sniff controller =  $6.57 \pm 1.94$  L/s, all comparisons with unassisted cough  $t(13) > -4.01$ ,  $p < 0.0015$ , all comparisons between methods of assistance  $t(13) < 1.15$ ,  $p > 0.27$  (Table II, Fig. 5). The mean PEF of automatic Sniff-Controller-FES assisted cough was  $23 \pm 27\%$  higher than coughing without assistance, and subjects self reported that the automatically stimulated cough was highly effective, and did not cause any discomfort. The mean FVC and MVV values after cough were  $3.01 \pm 0.11$  L and  $70.89 \pm 6.57$  L/min (3.5% and 9.3%), respectively. The methods of coughing did not affect MVV ( $F[4, 48] = 0.30$ ,  $p = 0.89$ ), and the effect on FVC was marginal ( $F[4, 52] = 2.54$ ,  $p = 0.051$ ).

#### IV. CONCLUSION/DISCUSSION

Experiments in 16 able-bodied participants allowed us to identify the precise point of glottis closure using the sniff-controller, and experiments in 14 subjects with SCL verified that the sniff controller can effectively time and trigger FES-induced cough. A key novel feature of this study was the synchronized measurements of nasal airflow with endoscopic video of cough events. This contributed a compelling demonstration of the process of glottis closure and its relationship to nasal airflow and neck and abdominal muscle contraction. It was this combination that allowed us to identify the critical time-point and duration for FES activation. This also provided for several novel observations, such as the neck muscle

contraction that started before the abdominal muscles contraction and glottis closure during cough. This may reflect an accessory muscle contribution to the inspiration that precedes cough.

All assistive methods tested in this study improved cough efficacy compared to unassisted cough by about 25%, and reached about 76% of the mean expected values of PEF based on European Respiratory Society standards of able-bodied people ( $8.78 \pm 0.75$  L/s) [38]. Here these values were obtained by delivering current through two large abdominal surface electrodes. This configuration of stimulation electrodes provides extensive coverage, and minimizes the need for accuracy in placement. That said, this study was aimed at examining sniff-controlled triggering of FES and not electrode design and placement. Thus, we varied method of triggering across conditions but kept the electrodes constant. It is conceivable that the large electrodes we used were perhaps less advantageous or convenient for some participants. Moreover, we did not titrate or systematically test the influence of the altered current density likely associated with this electrode configuration. Thus, we cannot make any statements as to any advantages or disadvantages associated with this electrode design. The issue of electrode design and placement should be further studied separately [39], and here we can make conclusions solely regarding methods of triggering. Indeed, given the current results with surface electrodes, we speculate that the sniff-controller can be equally used to accurately time and trigger other methods for stimulation and cough induction, such as spinal epidural electrodes [40], microstimulators [41] or magnetic stimulation of the thoracic nerve roots [42], [43].

There are several methods to self-trigger FES. Alternatives range from a simple button, to chin-joystick activation [19], and to EMG signals obtained from either the pectoralis major muscle or the deltoid muscle [20]. Furthermore, our approach is not the only one to trigger FES off the respiratory trace itself [23]. Initial efforts in this direction used the signal obtained from a full-mask spirometer [25], and it was hypothesized that modifications in the ensuing FES output would allow its application for chronic use [26]. Whereas a full-mask spirometer may be considered obtrusive, an important modification has been the extraction of the respiratory trace from plethysmographic belts and its application to FES triggering for both assisted ongoing respiration and assisted cough [27], [28]. Each of these methods has its advantages and disadvantages. Triggering off plethysmographic belts is very attractive because these are the least obtrusive of the methods tested. The value of this advantage cannot be overstated. In turn, a direct comparison implies that plethysmographic belts provide a less sensitive measure of airflow events [44], and they cannot account for transient events of paradoxical breathing where the chest and abdomen reverse direction in relation to inhalation and exhalation, a common occurrence in able-bodied and paralyzed individuals alike [45], [46]. Indeed, given these issues, to the best of our knowledge FES triggering by plethysmographic belts has yet to be tested in SCL patients. The disadvantages of the sniff-controller presented in this study are first and foremost its esthetic quality. A nasal cannula has the “look of disease,” and it will not be readily worn by

users in public. This largely restricts its application to sessions dedicated to coughing in privacy, and limits/prevents its application as an assistive tool for ongoing respiration (except perhaps in a hospital rehabilitation setting). Moreover, the sniff-controller method will likely fail all together in cases of a completely stuffed nose. Given that a stuffed nose is more likely exactly at times where cough is more important, this is a meaningful weakness. Finally, for the sake of consistency with most other studies, here we applied FES in the supine position. Although several studies imply only minimal differences in FES outcome as a function of posture [39], [42], such differences may nevertheless materialize because abdominal muscle length is slightly increased supine compared with seated [47]. Thus, the influence of posture on sniff-triggered FES remains to be investigated. In turn, the advantages of the method presented in this study are its simplicity (hence potential low cost if commercialized), its robustness, and its temporal accuracy. Moreover, patients with all levels of paralysis can independently activate the system. This provides for a critical component of independence and freedom from caregiver. Finally, and critically, we demonstrated that it works in paralyzed individuals. Indeed, several subjects in this study noted the added privacy and independence that this system affords, and also spontaneously subjectively stated that using the sniff-controlled system they experienced the "best" cough they remember in years since injury. With this in mind, we conclude that future developments aimed at developing a smaller wireless nasal sensor to replace the nasal cannula may provide for an optimal sniff-controlled system that will be used by patients in need.

## APPENDIX

### *The Sniff Controller-FES Device Code*

```
// ===== Define pins
=====
const int ledPin = 13;
const int analogInPin = A6; // Analog input pin
const int startPin = 2; // Red Button
const int pulsePin = 3; // Output pin
const int manualPin = 4; // Monitors manual pin status can
be LOW or HIGH – Stimulation mode
const int sniffPin = 5; // Standby mode activation – Sniff /
Button mode

// ===== Define pulse
parameters =====
const int pulseDelay = 50; // in ms
const int pulseFreq = 100; // in Hz
const int pulseDuration = 500; // in ms
// ===== Define Cough Detection
Parameters =====
const int timer = 1; // The time scale of the data from the
sensor
const int duration = 40; // Time window to detect the
cough 40 points = 58-59 ms
const int length = duration / timer; //Time window
translated to ms

const int length2 = 4; // inhale verification – short length to
catch the spike
// (To know that you are below a minimum)
- set to zero to cancel this test
const float meanx = ( (float(length) / 2) - 1 ) / 2; //constant
number for the mean value of x, depends on length
const float tb1 = -4; // slope b threshold, for fast glottice
closure
// ===== Define
vairiables =====
int memory[length]; //Will save last sensor data
int counter = 0; //Used to save last point that data was saved
float varx = 0; //saves the variance of x
float meany1 = 0; //saves the mean y value in the last 40 ms
float meany2 = 0; //saves the mean y value in the last 4 ms
float b1 = -100; //saves current slope
float b1_old = -100; //save last slope

unsigned long ADCTimer = 0; //used to save current time
const int ADCDt = 20; // scan interval
int analogIn = 440; //saves last analog in for sniff detection
int analogInOld = 440; //saves last analog in for sniff
detection
const int upperThreshold = 500; //upper threshold for sniff
detection
int sniff = 0; //Detected sniff in the
int sniffOld = 0; //Was sniff detected last scan time
(ADCDt)
unsigned long sniffTimer = 0; //used to store time from last
sniff
const int tShort = 2000; // time interval two short sniffs
should occur
int STATE = 1; // Saves the state of the systme State = 1 –
manual, State = 21 – Sniff, State = 22 – Button
int coughDetection = 0; //should go to sniff Detection state
int coughTrigger = 0; //should trigger cough
// =====
=====
// Function to setup communication
// The function also sets up varx – variance of uniform
variable (1, length)
void setup() {
// initialize serial communications at 9600 bps:
Serial.begin(9600);
pinMode(pulsePin, OUTPUT);
pinMode(ledPin, OUTPUT);
pinMode(startPin, INPUT);
pinMode(manualPin, INPUT);
pinMode(sniffPin, INPUT);
digitalWrite(pulsePin, LOW);
digitalWrite(startPin, HIGH);
digitalWrite(manualPin, HIGH);
digitalWrite(sniffPin, HIGH);
digitalWrite(ledPin, HIGH);
for (float i = 0; i < (length / 2); i++) {
varx += pow(i - meanx, 2);
};
}
```

```

    varx = varx / (length / 2);
}

// Function that sets the state of the box in each iteration of
the main loop of the controller
// State machine model
void setState(){
    if (digitalRead(manualPin) == LOW) {
        STATE = 1;
    }
    else { //(digitalRead(manualPin) == HIGH
        if (digitalRead(sniffPin) == LOW) { //manual pin is off
            sniff pin is on
                STATE = 21;
            }
        if (digitalRead(sniffPin) == HIGH) { //manual pin is off
            sniff pin is off
                STATE = 22;
            }
        }
    Serial.println("");
    Serial.print(STATE);
    Serial.print(" ");
    Serial.print(coughDetection);
}

// A function to print out the log while monitoring the sniff
device
// Prints out to screen the state of several variables
void printToLog() {
    for (int i = 0; i < length; i++) {
        Serial.print(memory[i]); //prints the readout of the device
        Serial.print(" ");
    }
    Serial.println("");
    for (int i = 0; i < (length/2); i++) {
        Serial.print(memory[(counter + 1 + i) % length]);
        Serial.print(" ");
    }
    Serial.println("");
    for (int i = 0; i < (length/2); i++) {
        Serial.print(memory[(counter + (length/2) + 1 + i) %
length]);
        Serial.print(" ");
    }
    Serial.println("");
    Serial.print(counter);
    Serial.print(" ");
    Serial.print(meanx);
    Serial.print(" ");
    Serial.print(varx);
    Serial.println("");
    Serial.print(meany1);
    Serial.print(" ");
    Serial.print(meany2);
    Serial.print(" ");
    Serial.print(b1);
    Serial.print(" ");
    Serial.println(b1_old);
}

// ===== Main loop of
the controller =====
void loop() {
    while (1) { //main loop
        setState(); //sets the state of current iteration according
to the pin states

// This part is used for the simple function - on mode - red
button function
        if (STATE == 1) { //Manual mode
            // In initial stage, when manual pin is off only
            monitors start pin and manual pin
            while ((digitalRead(startPin) == HIGH)&(digital
Read(manualPin) == LOW)) { //Check red button triggering
or mode was changed
                }
            if (digitalRead(startPin) == LOW) { //Validate that
red button was pressed
                coughTrigger = 1; //Cough was triggered by
red button
            }
        }
        else if (STATE == 21) { //Monitor double sniff
            while ((coughDetection == 0)&(digitalRead(sniffPin)
== LOW) & (digitalRead(manualPin) == HIGH))
{ //checks that state did not change
                if ( ( millis() - ADCTimer) > ADCDt ) { //checks
that scan interval did not change
                    ADCTimer = millis(); //save current time
                    analogInOld = analogIn; //stores previous read of
the signal
                    analogIn = analogRead(analogInPin); //read new
signal
                    Serial.println(analogIn);

                    if ( ( analogIn > upperThreshold)&(analogInOld
< upperThreshold) ) { //did the signal cross the threshold?
                        sniff = 1; //sniff was detected
                    }
                    else {
                        sniff = 0; //sniff was not detected
                    }

                    if (sniff != 0) { //look for the second sniff
                        if ( ( ( millis() - sniffTimer) > tShort)&(sniffOld
!= 0) ) { //clears first sniff detection
                            sniffOld = 0;
                        }
                    }
                    if (sniffOld > 0) { //cough detection standby -
the system is ready for cough detection
                        coughDetection = 1;
                        sniff = 0;
                        sniffOld = 0;
                        Serial.println("Detect in 21");
                    }
                }
            }
        }
    }
}

```





- [12] R. Torres-Castro, J. Vilaró, R. Vera-Urbe, G. Monge, P. Avilés, and C. Suranyi, "Use of air stacking and abdominal compression for cough assistance in people with complete tetraplegia," *Spinal Cord*, vol. 52, pp. 354–357, May 2014.
- [13] W. D. Reid, J. A. Brown, K. J. Konnyu, J. M. Rurak, and B. M. Sakakibara, "Physiotherapy secretion removal techniques in people with spinal cord injury: A systematic review," *J. Spinal Cord Med.*, vol. 33, no. 4, pp. 353–370, 2010.
- [14] W. A. Choi, J. H. Park, D. H. Kim, and S. W. Kang, "Cough assistance device for patients with glottis dysfunction and/or tracheostomy," *J. Rehabil. Med.*, vol. 44, pp. 351–354, Apr. 2012.
- [15] T. A. Volsko, J. DiFiore, and R. L. Chatburn, "Performance comparison of two oscillating positive expiratory pressure devices: Acapella versus Flutter," *Respirat. Care*, vol. 48, pp. 124–130, Feb. 2003.
- [16] S. H. Linder, "Functional electrical stimulation to enhance cough in quadriplegia," *Chest*, vol. 103, pp. 166–169, Jan. 1993.
- [17] A. Zupan *et al.*, "Effects of respiratory muscle training and electrical stimulation of abdominal muscles on respiratory capabilities in tetraplegic patients," *Spinal Cord*, vol. 35, pp. 540–545, Aug. 1997.
- [18] U. Stanic, F. Kandare, R. Jaeger, and J. Sorli, "Functional electrical stimulation of abdominal muscles to augment tidal volume in spinal cord injury," *IEEE Trans. Rehabil. Eng.*, vol. 8, no. 3, pp. 30–34, Mar. 2000.
- [19] P. N. Taylor, A. M. Tromans, K. R. Harris, and I. D. Swain, "Electrical stimulation of abdominal muscles for control of blood pressure and augmentation of cough in a C3/4 level tetraplegic," *Spinal Cord*, vol. 40, pp. 34–36, Jan. 2002.
- [20] E. Spivak *et al.*, "Electromyographic signal-activated functional electrical stimulation of abdominal muscles: The effect on pulmonary function in patients with tetraplegia," *Spinal Cord*, vol. 45, pp. 491–495, Jul. 2007.
- [21] D. R. Gater, D. Dolbow, B. Tsui, and A. S. Gorgey, "Functional electrical stimulation therapies after spinal cord injury," *NeuroRehabilitation*, vol. 28, no. 3, pp. 231–248, 2011.
- [22] A. C. Guyton, "Pulmonary ventilation," in *Textbook of Medical Physiology*, H. Je, Ed., Philadelphia, PA, USA: WB Saunders, 1996, pp. 477–489.
- [23] H. Gollee, K. J. Hunt, M. H. Fraser, and A. N. McLean, "Abdominal stimulation for respiratory support in tetraplegia: A tutorial review," *J. Autom. Control*, vol. 18, no. 2, pp. 85–92, 2008.
- [24] E. J. McCaughey, A. J. McLachlan, and H. Gollee, "Non-intrusive real-time breathing pattern detection and classification for automatic abdominal functional electrical stimulation," *Med. Eng. Phys.*, vol. 36, pp. 1057–1061, Aug. 2014.
- [25] H. Gollee, K. J. Hunt, D. B. Allan, M. H. Fraser, and A. N. McLean, "A control system for automatic electrical stimulation of abdominal muscles to assist respiratory function in tetraplegia," *Med. Eng. Phys.*, vol. 29, pp. 799–807, Sep. 2007.
- [26] S. Salmons and J. C. Jarvis, "A control system for automatic electrical stimulation of abdominal muscles to assist respiratory function in tetraplegia," *Med. Eng. Phys.*, vol. 29, no. 10, pp. 1180–1181, Dec. 2007.
- [27] J. Sorli, F. Kandare, R. J. Jaeger, and U. Stanic, "Ventilatory assistance using electrical stimulation of abdominal muscles," *IEEE Trans. Rehabil. Eng.*, vol. 4, no. 1, pp. 1–6, Mar. 1996.
- [28] E. J. McCaughey, A. J. McLachlan, and H. Gollee, "Non-intrusive real-time breathing pattern detection and classification for automatic abdominal functional electrical stimulation," *Med. Eng. Phys.*, vol. 36, no. 8, pp. 1057–1061, 2014.
- [29] A. Plotkin *et al.*, "Sniffing enables communication and environmental control for the severely disabled," *Proc. Nat. Acad. Sci. USA*, vol. 107, pp. 14413–14418, Aug. 2010.
- [30] M. Knecht and T. Hummel, "Recording of the human electro-olfactogram," *Physiol. Behavior*, vol. 83, pp. 13–19, Oct. 2004.
- [31] T. Shimokawa, S. Yi, and S. Tanaka, "Nerve supply to the soft palate muscles with special reference to the distribution of the lesser palatine nerve," *Cleft Palate Craniofacial J.*, vol. 42, pp. 495–500, Sep. 2005.
- [32] J. Strutz, T. Hammerich, and R. Amedee, "The motor innervation of the soft palate. An anatomical study in guinea pigs and monkeys," *Eur. Arch. Oto-Rhino-Laryngol.*, vol. 245, no. 3, pp. 180–184, 1988.
- [33] J. Jakus, E. Halasová, I. Políacek, Z. Tomori, and A. Stránský, "Brainstem areas involved in the aspiration reflex: *c-fos* study in anesthetized cats," *Physiol. Res.*, vol. 53, no. 6, pp. 703–717, 2004.
- [34] J. Jakus *et al.*, "Brainstem circuitry of tracheal-bronchial cough: *c-fos* study in anesthetized cats," *Respirat. Physiol. Neurobiol.*, vol. 160, pp. 289–300, Feb. 2008.
- [35] M. Deschênes, A. Kurnikova, M. Elbaz, and D. Kleinfeld, "Circuits in the ventral medulla that phase-lock motoneurons for coordinated sniffing and whisking," *Neural Plasticity*, vol. 2016, p. 7493048, Apr. 2016.
- [36] T. Pantaleo, F. Bongianini, and D. Mutolo, "Central nervous mechanisms of cough," *Pulmonary Pharmacol. Therapeutics*, vol. 15, no. 3, pp. 227–233, 2002.
- [37] R. A. McBain, C. L. Boswell-Ruys, B. B. Lee, S. C. Gandevia, and J. E. Butler, "Electrical stimulation of abdominal muscles to produce cough in spinal cord injury: Effect of stimulus intensity," *Neurorehabil. Neural Respirat.*, vol. 29, pp. 362–369, May 2015.
- [38] "Standardized lung function testing. Official statement of the European respiratory society," *Eur. Respirat. J. Suppl.*, vol. 16, pp. 1–100, Mar. 1993.
- [39] J. Lim, R. B. Gorman, J. P. Saboisky, S. C. Gandevia, and J. E. Butler, "Optimal electrode placement for noninvasive electrical stimulation of human abdominal muscles," *J. Appl. Physiol.*, vol. 102, pp. 1612–1617, Apr. 2007.
- [40] A. F. DiMarco, K. E. Kowalski, R. T. Geertman, and D. R. Hromyak, "Spinal cord stimulation: A new method to produce an effective cough in patients with spinal cord injury," *Amer. J. Respirat. Critical Care Med.*, vol. 173, pp. 1386–1389, Jun. 2006.
- [41] V. W.-H. Lin, X. Deng, Y.-S. Lee, and I. N. Hsiao, "Stimulation of the expiratory muscles using microstimulators," *IEEE Trans. Neural Syst. Rehabil. Eng.*, vol. 16, no. 4, pp. 416–420, Aug. 2008.
- [42] M. I. Polkey, Y. Luo, R. Guleria, C. H. Hamnegard, M. Green, and J. Moxham, "Functional magnetic stimulation of the abdominal muscles in humans," *Amer. J. Respirat. Critical Care Med.*, vol. 160, pp. 513–522, Aug. 1999.
- [43] V. W. Lin, C. Hsieh, I. N. Hsiao, and J. Canfield, "Functional magnetic stimulation of expiratory muscles: A noninvasive and new method for restoring cough," *J. Appl. Physiol.*, vol. 84, pp. 1144–1150, Apr. 1998.
- [44] B. N. Johnson, C. Russell, R. M. Khan, and N. Sobel, "A comparison of methods for sniff measurement concurrent with olfactory tasks in humans," *Chem. Senses*, vol. 31, pp. 795–806, Nov. 2006.
- [45] A. De Troyer, M. Estenne, and W. Vincken, "Rib cage motion and muscle use in high tetraplegics," *Amer. Rev. Respirat. Disease*, vol. 133, pp. 1115–1119, Jun. 1986.
- [46] M. Estenne and A. De Troyer, "Relationship between respiratory muscle electromyogram and rib cage motion in tetraplegia," *Amer. Rev. Respirat. Disease*, vol. 132, pp. 53–59, Jul. 1985.
- [47] H. Rahn, A. B. Otis, L. E. Chadwick, and W. O. Fenn, "The pressure-volume diagram of the thorax and lung," *Amer. J. Physiol.*, vol. 146, pp. 161–178, May 1946.



**Lior Haviv** received the B.Sc. and M.Sc. degrees in chemical engineering and studied biophysics with the Ben-Gurion University of the Negev, Israel. He was a Researcher with the Human Olfaction Laboratory, Weizmann Institute of Science, Israel, and an Entrepreneur. He specializes in electronic nose and Research and Development of the Sniff controller as an Assistive Technology for people with disabilities.



**Hagit Friedman** received the M.Sc. degree in neurobiology from HUJI, Israel, and the Ph.D. degree in neurodevelopment and neuroimaging from T-IIT, Israel. She is currently a Researcher with the Department of Nursing, University of Haifa, Israel, specializing in neural development and rehabilitation.



**Uri Bierman** received the B.Sc. degree in biology from the Ben-Gurion University of the Negev, Israel. He also had attended a medical equipment course with Minhaltec College, Israel, from 2013 to 2014. He is currently a Researcher Assistant with Loewenstein Rehabilitation Hospital, operating research services for Prof. A. Catz, and is also the Medical Director and the CEO of Loewenstein Rehabilitation Hospital, Ra'anana.



**Itzhak Glass** received the B.Sc. degree in biology, the M.Sc. degree in zoology, and the Ph.D. degree in neurophysiology from Tel-Aviv University, Israel. He retired as the Director of the Institute of Neurophysiology, Loewenstein Rehabilitation Hospital. He is currently a Researcher of Neurophysiology.



**Vadim Bluvshstein** received the M.D. degree from the Pediatric Medicine Institute, Leningrad. He is currently the Director of the Urodynamics and Bladder Rehabilitation Unit, and a Senior Physician with the Spinal Rehabilitation Department, Loewenstein Rehabilitation Hospital, and also an Instructor with the Sackler Faculty of Medicine, Tel-Aviv University, Israel.



**Anton Plotkin** received the Dipl.Eng. degree in radio-communication and broadcast and television from Siberian State University, Russia, and the Ph.D. degree in electrical and computer engineering from the Ben-Gurion University of the Negev, Israel. He is currently the Director of Technology with Bluewind Medical Ltd., and is also with the Human Olfaction Laboratory, Weizmann Institute of Science, Israel.



**Elena Aidinoff** received the B.A. and M.A. degrees in psychobiology from Tel-Aviv University, Israel, and graduated in neuroscience from Stanford University, USA, and received the M.D. degree from the State Medical Institute, Sverdlovsk, Russia. She was an Associate Professor with the Helen Wills Neuroscience Institute, University of California, USA. She is currently the Acting Director of the Intensive-Care for Consciousness Rehabilitation Department, and formerly a Senior Physician with the Spinal Rehabilitation Department, Loewenstein Rehabilitation Hospital. She is also an Instructor with the Sackler Faculty of Medicine, Tel-Aviv University.



**Aharon Weissbrod** received the B.Sc. degree in electrical engineering from the University of Nevada at Reno, Reno, USA. He was with the Missiles Division, RAFEL M.O.D., as an Electronic Engineer. He is currently an Electrical Engineer, specializing in the design of electronic instruments for human olfactory system research, with the Human Olfaction Laboratory, Weizmann Institute of Science, Israel.



**Noam Sobel** received the B.A. and M.A. degrees from Tel-Aviv University, Israel, and the Ph.D. degree in neuroscience from Stanford University, USA. He is currently a Professor of Neurobiology with the Weizmann Institute of Science, Israel.



**Sagit Shushan** received the M.D. degree from the Ben-Gurion University of the Negev, Israel. She was a Researcher with the Human Olfaction Laboratory, Weizmann Institute of Science, Israel, and an Ear, Nose, and Throat Surgeon with the Wolfson Medical Center. She specializes in rhinology and human olfaction disorders.



**Amiram Catz** received the M.D. degree from the Hadassa Medical School, Hebrew University, Jerusalem, and the master's degree in health-administration and the Ph.D. degree in physiology from Tel-Aviv University, Israel. He is currently a Professor of Rehabilitation with Tel-Aviv University, the Medical Director and the CEO of Loewenstein Rehabilitation Hospital (LRH), Ra'anana, and the Director of the Spinal Rehabilitation Department with LRH.