

Transferrable Expertise From Bionic Arms to Robotic Exoskeletons: Perspectives for Stroke and Duchenne Muscular Dystrophy

Kostas Nizamis¹, Arno H. A. Stienen, Derek G. Kamper, Thierry Keller, Dick H. Plettenburg, Elliott J. Rouse²,
Dario Farina³, Bart F. J. M. Koopman⁴, and Massimo Sartori⁵

(Invited Paper)

Abstract—Upper extremity function is affected by a variety of neurological conditions. Robotic exoskeletons offer a potential solution for motor restoration. However, their systematic adoption is limited by challenges relative to human intention detection and device control. This position article offers a focused perspective on this topic. That is, on how knowledge gained from the design and implementation of human-machine interfaces (HMIs) for bionic arms can benefit the field of rehabilitation exoskeletons. Three broadly used HMIs in bionic arms are here investigated, including surface electromyography, impedance, and body-powered control. We propose that combinations of these HMIs could push forward upper extremity exoskeleton development. In this context, we provide concrete applicative examples in two selected clinical scenarios, including post-stroke and Duchenne muscular dystrophy individuals. The discussed solutions can open new avenues for the translation of robotic exoskeletons in a large set of clinical settings and enable a class of exoskeleton technologies that could support a broader range of impairment and disease types.

Index Terms—Bionic arms, Duchenne muscular dystrophy, robotic exoskeletons, stroke, upper limb.

Manuscript received February 27, 2019; revised April 13, 2019; accepted April 17, 2019. Date of publication April 22, 2019; date of current version May 16, 2019. This paper was recommended for publication by Associate Editor S. Micera and Editor P. Dario upon evaluation of the reviewers' comments. This work was supported in part by the Flextension Foundation through the Netherlands Organization for Scientific Research (NWO), in part by the Duchenne Parent Project, in part by Hankamp Rehab, in part by Spieren voor Spieren, in part by TMSi, in part by Festo, in part by Pontes Medical under Project 13525, and in part by ERC Starting Grant INTERACT under Grant 803035. (Corresponding authors: Kostas Nizamis; Massimo Sartori.)

K. Nizamis, B. F. J. M. Koopman, and M. Sartori are with the Department of Biomechanical Engineering, Technical Medical Centre, University of Twente, 7522 NB Enschede, The Netherlands (e-mail: k.nizamis@utwente.nl; m.sartori@utwente.nl).

A. H. A. Stienen is with the Department of Physical Therapy and Human Movement Sciences, Northwestern University, Chicago, IL 60611 USA.

D. G. Kamper is with the Joint Department of Biomedical Engineering, North Carolina State University, Raleigh, NC 27695 USA.

T. Keller is with the Neurorehabilitation Area at the Health Division, TECNALIA, E-20009 San Sebastian, Spain.

D. H. Plettenburg is with the Department of Biomechanical Engineering, Delft University of Technology, 2628 CD Delft, The Netherlands.

E. J. Rouse is with the Department of Mechanical Engineering, University of Michigan at Ann Arbor, Ann Arbor, MI 48109 USA.

D. Farina is with the Department of Bioengineering, Imperial College London, London SW7 2AZ, U.K.

Digital Object Identifier 10.1109/TMRB.2019.2912453

I. INTRODUCTION

THE ABILITY to perform coordinated arm-hand movements relates to the quality of life, as well as to social participation and acceptance [1]. As we manipulate objects primarily through our hands, neurological injuries and disorders affecting the upper extremity [1] highly impair one's ability to interact with the external world. In this context, robotic exoskeletons have been long developed for restoring impaired motor functions [2], [3], due to their potential in promoting active user participation [4], independence [5] and potential suitability for home rehabilitation [6].

The research field of robotic exoskeletons has been growing rapidly [2], [3], [7], resulting in an explosion of wearable assistive and rehabilitation technologies [8]. However, demonstrated functional and clinical impact is still limited. Kinematic compatibility and the additional weight imposed on the existing limb by a robotic exoskeleton are important factors limiting robotic exoskeleton use. The development of soft exosuits, aims to easier fitting and lightweight designs that require less energy to use [9], [10]. Additionally, the lack of a rigid frame simplifies sensor placement, and prevents extra strains to the body of the user. However, soft exosuits result in a limited amount of support compared to rigid robotic exoskeletons [9]. Bos *et al.* [3] identified forty-six hand exoskeletons intended for use as daily assistive devices, yet most of them did not reach the market. Moreover, Maciejasz *et al.* [7] concluded that the results of the clinical evaluation of robotic exoskeleton-aided therapy are sparse. Additionally, despite the large research performed in the last 30 years [11], the effectiveness of robotic therapy over conventional physiotherapy is modest [7], [12], especially in people with neuromuscular injuries (e.g., stroke) or progressive impaired function (e.g., Duchenne Muscular Dystrophy or DMD). Important causes are the slow translation of robotic exoskeletons from laboratories to clinical setting, where clinical trials can further assess their efficacy [7], and the fact that the broad use of exoskeletons for daily or home use has not been consistently translated from the laboratory to the clinic [13]–[15]. Additionally, the lack of natural and intuitive human-machine interfaces (HMI), presents an important challenge for the future, indicating that the use of robotic exoskeletons in the real world requires significant improvements before it can be realised [5], [16].

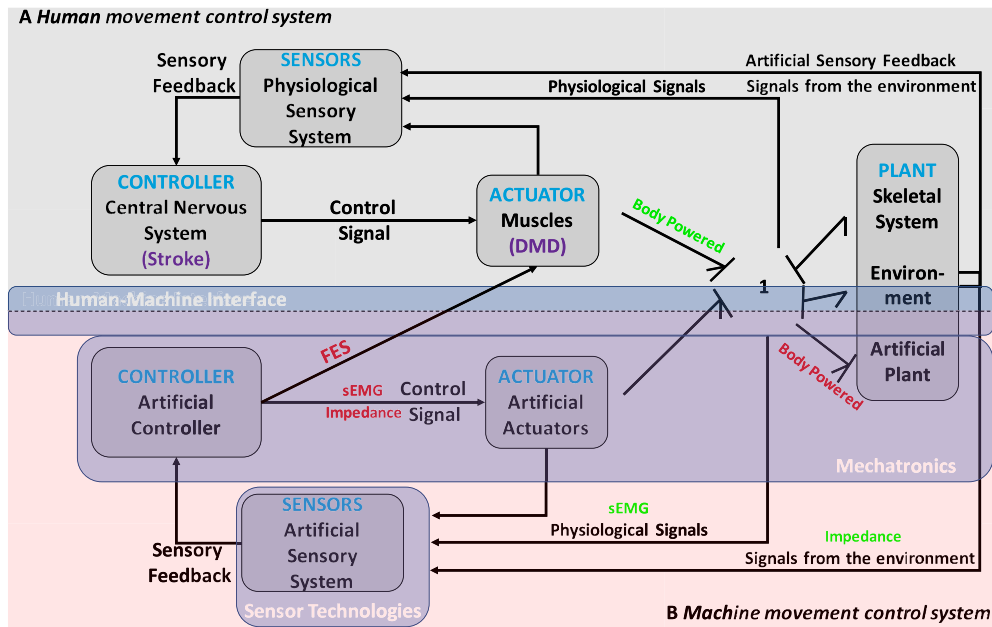


Fig. 1. This figure illustrates A) the human movement control system together with B) the machine movement control system. The machine movement control system can be a robotic exoskeleton or a bionic limb. With purple are noted the two clinical cases discussed in this article. DMD affects the muscles, and stroke causes central nervous system disorders. With red and green we can see the interaction between each of the three human-machine-interfaces discussed and the human, plus functional electrical stimulation (FES). The input signal (motor intention detection) and the resulting interaction are noted in green and red, respectively. The three major components of bionic limbs and robotic exoskeleton systems are highlighted in the machine movement control system. The mechatronics consist of the controller, actuator and the device (bionic limb or robotic exoskeleton), the sensor technologies refer to the artificial sensory system and the human-machine interface represents the flow of information between the human movement control system and the machine movement control system. Modified from [42].

On the other hand, the field of bionic arms has undergone substantial scientific and technological advances with direct clinical and market impact [17]. Prosthetic procedures, such as targeted muscle re-innervation (TMR) [18] and osseointegration, greatly improved surface electromyography (sEMG)-based decoding and device control [19] as well as donning/doffing [20] and stability of the bionic arms fixation. Such procedures have opened up new opportunities for HMI. In the case of people with brachial plexus injury, where a robotic exoskeleton would be the preferable (minimally invasive) technology, elective amputation and use of a bionic arm is sometimes preferred [21]. In this way, people with critical injuries can substitute a non-functional limb with a highly functional bionic limb, indicating that bionic technology is more mature to enhance functional recovery.

Robotic exoskeletons such as the MyoPro elbow/wrist/hand orthosis [22], [23] and the SaeboGlove [24] are commercially available. However, in terms of HMIs, they are less advanced compared to commercial bionic limbs, which are driven by pattern recognition myocontrollers [25], [26] or biomechanical models [27], enabling multiple degrees-of-freedom (DOF).

Given the close relation and overlap between bionic arms' and robotic exoskeletons' HMIs (see Section II), this article proposes a focused perspective for how expertise and technological advancements in bionic arms could be translated to the developing field of arm-hand exoskeletons. We trust that the development of such a roadmap will lead to a new class of wearable robots that can seamlessly cooperate as a natural extension of the human body.

In this article, we first introduce three key technologies well established in current HMIs for bionic arms including

sEMG, impedance and body-powered control. Second, we propose how HMIs can be translated to exoskeletons. Third, we introduce relevant clinical scenarios that can benefit from the use of exoskeletons, including stroke and DMD. These key scenarios allow distinguishing between exoskeletons used for rehabilitation or restoration (i.e., stroke scenario) and those used for functional replacement, i.e., assistive technologies for daily use (i.e., DMD scenario). Finally, we discuss how these technologies can be combined in order to be used for the presented clinical scenarios. This provides new perspectives on how exoskeletons can be interfaced to individuals with neuromuscular impairments.

II. FOCUSED PERSPECTIVE

A. Learning From Bionic Arms

Research on prosthetic arms goes back for centuries [28], reaching a strong impact on the market [29]. Arm exoskeletons share a similar design and functional features to current bionic arms, yet underline unique and distinctive attributes, i.e., exoskeletons act in parallel to the impaired limb, rather than replacing it. Fig. 1 shows differences at the HMI level across bionic arms and exoskeleton technologies. The human movement control system (Fig. 1, A) and the machine movement control system (Fig. 1, B) act in parallel to each other for exoskeletons but in series for bionic arms. In this context, we argue that the transfer from bionic arms to exoskeletons should focus on the HMI level.

The term HMI refers to methodologies for the identification of the user's intent to move from biological signals (i.e., surface electromyograms or sEMG) or body force and position

data and its translation into robotic commands. Numerous invasive [30], [31] and non-invasive [32]–[37] interfaces were developed in the past and applied to both bionic arms [30]–[34], [36], [37] and exoskeletons [35], [38]–[41].

There are different levels of interfacing with the human [42] (Fig. 1). Myocontrolled bionic arms [32], [33] interface with residual muscle tissues replacing the missing limb. There are also bionic lower limbs that interface with the musculoskeletal plant via impedance control [34], [35] (utilising the interaction between the user and the robotic limb) or via body-powered control [36], [37] (by using an intact limb to mechanically control a bionic limb). Neuroprostheses are available to stimulate muscles or nerves [30], [31] to elicit movement in the impaired limb.

B. Clinical Scenarios

In this position article, we rely on two representative key clinical scenarios including stroke [43] and DMD [44]. For both scenarios there is a clear need for active support and robotic exoskeletons present a feasible solution. However, despite this similarity both conditions present clear differences at the HMI level. Stroke represents a class of conditions where the affected individual needs to re-learn how to use their limbs, thus requiring HMIs providing minimal assistance in order to facilitate motor learning. On the other hand, muscular dystrophies are characterized by a progressive loss of muscle strength, with no potential for motor function restoration, thus requiring HMIs providing maximal assistance to postpone tissue degeneration. By discussing extensively those distinct neuromuscular deficiencies we cover a large HMI spectrum which, if addressed properly, would enable a class of exoskeleton technologies that could support a broader range of impairments and disease types.

Stroke: It is caused by a lesion in the central nervous system or CNS and results in loss of motor capacity [43]. According to a recent study by the world stroke organization, it has an incidence of 35–909 per 100,000 people per year worldwide [45] and the observed acceleration in the ageing population is expected to raise these numbers [45]. Stroke results in motor impairment with a level of similarity to other neurological conditions including multiple sclerosis (MS) [46] and spinal cord injury (SCI) [47], i.e., early fatigue onsets, spasticity, paresis, muscle contractures and rigidity, reduced mobility and musculoskeletal coordination and mechanical tissue changes [48]. Hence, exoskeleton technologies effectively supporting stroke rehabilitation could have a broader impact on other clinical scenarios, i.e., SCI and MS.

Exoskeletons targeting stroke individuals are designed for rehabilitation of the impaired motor function [8]. Currently, static splints are used for increasing range of motion and preventing contractures [49]. However, although highly prescribed by doctors, these are reportedly ineffective [50] and uncomfortable for long-term use [51]. Active exoskeletons are also broadly for clinical or home rehabilitation [3].

For stroke patients, exoskeletons are controlled via assistance-as-needed strategies to enable the active participation of individuals during the rehabilitation process [52], [53].

DMD: It is an X chromosome-linked progressive neuromuscular disease which leads to physical disability and shortened life expectancy [54]. There is currently no therapy developed for DMD. Nevertheless, recent technological advances have significantly increased the life expectancy of people with DMD [55]. Due to this fact, the population of individuals with DMD is expected to significantly increase in the near future [56]. DMD presents a representative case for other existing muscular dystrophies as it is the most common and severe form of muscular dystrophy [57], with an incidence of 1 out of 4,000 male births [58].

People with DMD need exoskeletons to maintain tissue integrity. This can be achieved by the decrease of detrimental mechanical load on their muscle tissues in order to minimise contractures and joint deformities that develop due to disuse of the limb [59]. There is evidence that people with DMD can greatly benefit from the use of arm exoskeletons [60], thereby promoting the use of the upper limb. Even more importantly, DMD individuals need devices to assist function in daily living for a prolonged period of time [61]. Regarding the hand, the only exoskeletons systematically adopted in people with DMD are passive splints [62]. These aim at maintaining a large active range-of-motion for the fingers and the wrist and slow the development of contractures.

Muscular dystrophies present a different scenario than stroke as the disease is progressive. While short-term therapeutic benefits may be seen with the use of a device, the primary focus is on providing as much assistance as possible. Thus, the exoskeleton should minimise the effort of the user to enable activities of daily living.

C. Key Technologies in Human-Machine Systems

Whether for exoskeletons or bionic arms, an HMI should enable the robust identification of the user's movement intent and translate it into machine commands. In the remainder of this section, we introduce three HMI technologies as well as the use of functional electrical stimulation (FES), which we selected for their potentials. These selected technologies will be combined together in Section III to compose HMIs specifically tailored for stroke and DMD.

sEMG Control: Myocontrol is broadly used in bionic arms [63], [64]. Direct sEMG control [65] is typically combined with co-contraction to enable switching across DOF. However, it has been reported as an unintuitive approach providing limited gains in functionality [64]. More advanced approaches rely on two main techniques [66]. The first is model-free machine learning [67]. The second emerging one is the model-based approach using musculoskeletal modelling [68]–[71]. Machine learning uses multi-channel sEMG recordings in conjunction with model-free algorithms in order to achieve higher functionality and control over more DOF. In this context, pattern recognition [72] (classifying a finite number of movements based on features of the sEMG signals) and regression [73] (continuous mapping of sEMG signals to kinematic variables) are currently used for the control of bionic arms. However, training in a specific spatiotemporal condition using machine learning does not necessarily translate into another [74]. The combination

of such approaches with biomechanical models can overcome this limitation [68], as recently demonstrated [69], [70].

Pros and Cons: The benefit of myocontrol techniques is that they allow for the user's intent to be detected before the movement actually takes place and even if no mechanical movement is possible [68]. This way, it is possible to synchronise the actual muscle contraction to the movement of a device, thus making the combined movement more intuitive [64]. On the other hand, sEMG can be contaminated by electromagnetic interference, skin perspiration and fatigue [75], and movement and crosstalk artefacts [76]. The use of sophisticated machine learning techniques is reportedly low for more challenging 'outside the lab' conditions [64] as it requires significant set-up and training time. Also, myoelectric bionic arms tend to be rejected by the user due to unpredictability in their response [77].

Impedance Control: Impedance and admittance control govern the relationship between position and force (torque) rather than controlling either position or force explicitly, where admittance is the inverse of impedance. The impedance control approach was originally proposed by Hogan [78] and has had widespread success in wearable robotic technologies for the lower extremity. For example, Herr *et al.* have used impedance control to govern the behaviour of their bionic ankle and knee, which have had promising clinical results [76], [77]. Furthermore, Goldfarb *et al.* have implemented impedance control in their robotic leg, which has provided a rich foundation of work on the development of many aspects of robotic legs [81], [82]. Impedance control is particularly useful for lower extremity bionic limbs because it permits mechanical dynamics between the body centre of mass and the ground, governed by the multi-joint mechanical impedance of the robotic hardware. Thus, impedance control circumvents the use of high-gain position-controlled mechanisms, which would cause the wearer to 'ride' the robotic leg or exoskeleton. This approach contrasts the control of upper limb robotics; bionic arms have traditionally used muscle sEMG as a command signal, which often controls the velocity of the joint or grasp mode [33], [83], [84].

Pros and Cons: One unique characteristic of impedance-based control schemes is that they enable mimicking the compliance of the musculoskeletal system. Knowledge of how impedance is regulated during movement forms the foundation of a biomimetic impedance control approach, which can be implemented in the control of exoskeletons and bionic arms. The impedance control framework is the only control strategy that permits the ability to match human regulation of kinetics, kinematics, and impedance, simultaneously. However, further studies are needed to ascertain the value of the biomimetic impedance framework, both in bionic limbs and exoskeletons. This case is dominated by lower extremity bionic limbs. Upper extremity bionic limbs are stiff mechanisms controlled using sEMG thresholding or pattern recognition. The work from Keemink *et al.* [85], recently addressed the cons of admittance control and provided a comprehensive and complete admittance controller framework, that can be used for physical human-robot interaction and enhance user tailored control.

Body-Powered Control: To control a bionic arm, it is important that the user can provide a proper feedforward signal. Equally important is that the user receives a proper feedback signal. This was already pointed out by Wiener in 1948 [86]. The human hand has excellent control; there is a wealth of effectors and of afferent information (muscle spindles and Golgi-tendon organs) providing excellent (proprioceptive) feedback. In body powered bionic arms, shoulder movements are most commonly harnessed to provide the intent of the motion. The shoulder muscles involved provide proprioceptive feedback. The bionic arm user can learn how the position of the shoulder and/or the upper arm at the unaffected side is a measure for the opening width of the bionic arm. Equally, the user can learn to interpret the forces perceived on the shoulder as a measure for the applied pinch force of the bionic arm.

Existing control methods include harnessing body movements, cineplasty [87], muscle bulging [88], myoelectricity, and myo-acoustics [89]. New control methods explored include peripheral nerve interfaces [90] and brain-computer interfaces [91].

Pros and Cons: Given the need for feedback, only harnessing body movements, cineplasty, and peripheral nerve interfaces are feasible control methods. Research in body-powered bionic arms focusses on lowering the operating forces to enhance force and displacement perception. For all options, the design of a servo mechanism is instrumental [92]. All that is said for bionic arms applies to robotic exoskeletons as well – it is all about how a human being can control a machine. Closed-loop control is also a necessity here. However, body powered prosthesis, are quite limited in the number of DOFs that they can restore and actively control.

Functional Electrical Stimulation (FES): FES is broadly used together with robotic exoskeletons [93]–[96]. Transcutaneous FES is integrated with exoskeletal structures in which the exoskeleton takes a double function: i) it carries the electrodes; ii) it stiffens or stabilises the joints that cannot be well controlled by FES alone. A typical example of such a transcutaneous FES upper extremity exoskeleton is the Bioness Inc. H200, a device that has been used in clinical applications for almost two decades. Current challenges for the seamless integration of all these technologies into an intelligent exoskeleton for unassisted hand grasp are mainly on the material side on stretchable electronics, the electrode-skin interface, and personalisation.

Pros and Cons: For the upper limb, recent reviews concluded that FES is a promising technology for rehabilitation in combination with robotic exoskeletons [97] and that FES systems reduce spasticity and improve the range of motion and the quality of life of people with stroke [98]. To the authors' best knowledge, there is no evidence of FES being used with individuals with DMD to assist in functional movements of the upper limb. However, there are studies [99]–[101] on the therapeutic effects of FES for people with muscular dystrophies, but with controversial and sometimes contradicting results. It is therefore important to approach this idea with the appropriate caution since it is known from the literature that exercises imposing high mechanical stress and

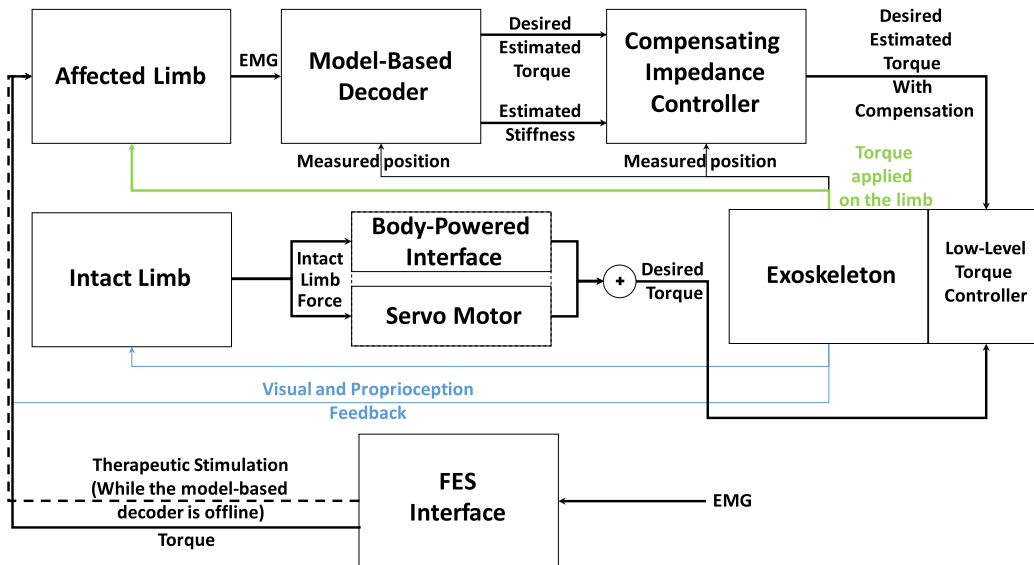


Fig. 2. This figure illustrates the proposed control diagram for stroke, including a body powered interface together with sEMG and impedance. All the separate elements are described in detail in Section III.

eccentric muscle contractions can be harmful to individuals with DMD [102].

III. THE PROPOSED POSITION

In the previous sections, we described three key HMI components currently used in bionic arms (sEMGs, impedance control and body-power schemes) and neuro-prostheses (FES). Here, we discuss our position regarding their combined use and translation into robotic exoskeletons as an intervention for the clinical scenarios discussed previously.

Position for Stroke Case-Scenario: Fig. 2 shows the conceptual design of a stroke-specific HMI scheme. The user intent is estimated by means of sEMG from the affected limb [32], [33]. In stroke patients with residual proprioception [103], this provides a level of closed-loop control. The sEMG signals are directed together with position information from the robotics exoskeleton to a model-based decoder [19], which provides an estimate of the desired torque in the limb's joints. This allows the implementation of control strategies in which the subject is supported as little as needed and proportionally to residual force, central for neuroplasticity [64]. Moreover, this allows the estimation of joint stiffness, as previously shown, and therefore establishes closed-loop controllers operating in the impedance/admittance domain [104]. An impedance compensation controller receives the estimated torque and stiffness from the model and also position information from the exoskeleton. In this way, it can be directly controlled from the sEMG-decoded stiffness and compensate for altered joint mechanics due to tissue structural changes [48], [104]. This can be achieved by a position-based compensator. The impedance compensation controller needs to be calibrated beforehand in order to compensate for joint-stiffness induced torques, similar to the active stiffness compensation proposed by Lobo-Prat *et al.* [105]. Additionally, the impedance compensation controller can be

used to provide active gravity compensation including weight compensation of handheld objects [105], or manipulate the virtual dynamics of the device and add an extra level of control customization [106]. The final desired estimated torque is directed to a low-level torque controller and the outcome torque is applied to the limb by the exoskeleton. For individuals with hemiparesis, body-power technology can be used to harness the functionality of the non-impaired side and further enhance the active participation of the user. In the case of more impaired subjects, the torque provided by the non-impaired limb can be amplified by the addition of a servo motor (Fig. 2). In this case, the desired torque is also directed to a low-level torque controller and the outcome torque is applied to the limb by the exoskeleton. We propose the use of electrical stimulation (ES) as a means to improve upper limb functionality by reducing muscle contractures and spasticity while improving coordination [107]. This is also reported to happen in cases of MS [108] and SCI [109], however for the lower limb. With such use of FES, we can optimise the use of the robotic exoskeleton by the human.

Position for DMD Case-Scenario: Fig. 3 shows the DMD specific HMI scheme. Similar to what we proposed previously for stroke, the user and the robotic exoskeleton interface by the means of sEMG of the affected limb. Closed-loops sEMG control is achievable in DMD with residual proprioception [110]. We propose to combine sEMG with a virtual impedance/admittance model similar to [106], [111]. sEMG signals are directed together with position information from the robotic exoskeleton to a time-varying model-based decoder [19], which estimates the desired torque in the limb's joints. The model-based decoder adapts with time (time-varying) to the progress of the disease. This can be done via multi-scale mechanobiology models characterising cellular-to-organ scale musculoskeletal adaptations [112], [113]. The impedance compensation controller will receive the estimated torque and stiffness from

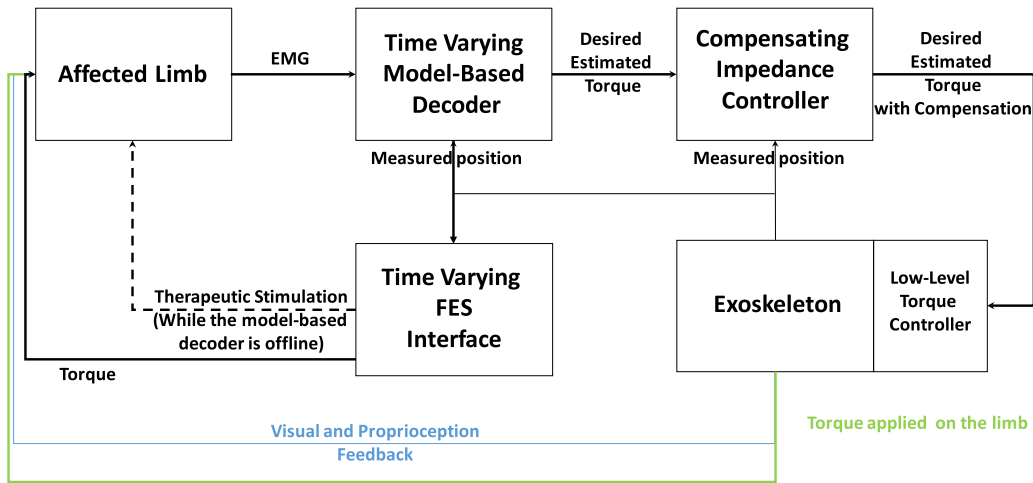


Fig. 3. This figure illustrates the proposed control diagram for DMD. In this case, we combine sEMG with a time-varying biomechanical model (due to the progressive nature of the disease) and impedance control. All the separate elements are described in detail in Section III.

the model and also position information from the exoskeleton. This can be achieved by a position-based compensation similar to the one applied to abnormal joint stiffness induced forces by Lobo-Prat *et al.* [106]. The impedance compensation controller needs to be calibrated beforehand in order to compensate for such parasitic forces and torques, due to abnormal joint stiffness [106]. Additionally, the impedance compensation controller can be used to provide active gravity compensation [105] or manipulate the virtual dynamics of the device in order to add an extra level of control customization for the user [106]. The torque estimated by the model-based sEMG decoder is algebraically added to the torque estimated from the compensatory impedance controller and will be sent to the low-level torque controller. The outcome torque will be applied by the exoskeleton to the affected limb.

The therapeutic ES will act when the sEMG-impedance hybrid is offline. The interaction between the sEMG model-based decoder and the ES module will have a dual nature. First, it tells the ES module how much exercise is needed based on the quality of the sEMG measurements. Second, it will indirectly affect the performance of the model-based decoder by improving muscle quality. The ES module can be integrated into the robotic exoskeleton to enhance portability.

IV. DISCUSSION

This position article presents two HMI designs for addressing distinctive clinical scenarios including stroke and DMD. For both scenarios, the proposed designs include different combinations of sEMG, impedance control, and body-powered technology in combination with FES. The technologies discussed in this article covered three crucial objectives for the control of bionic limbs: 1) the connection to the human body (sEMG) 2) the control of actuators (impedance/admittance) and 3) usage of the residual limb capabilities (body-powered). In this context, FES enables establishing neuroprostheses for upper extremity function restoration as a stand-alone [107] or in combination with a robotic exoskeleton [114]. Therefore, FES is the optimal

starting point for investigating new concepts of integration between bionic prosthetics and robotic exoskeleton technologies. The HMI type considered in our position article aims to operate at a lower level than cognitive HMIs. Our proposed HMIs aim to interface wearable robots with the human neuromuscular system via the recording and processing of bio-electrical information.

Additional HMI technologies exist that were not covered by this article [42], [115]. Common non-invasive HMIs include brain-computer interfaces like electroencephalography [116] (EEG), and near-infrared spectroscopy [117]. At the muscle level, interfaces like mechanomyography [89] and sonomyography [118] aim at providing alternatives to sEMG. Last but not least, HMI such as eye tracking, tongue interfaces and joysticks have been heavily used for the control of bionics [42]. Those have a clear disadvantage of sacrificing one function to support another.

In addition to HMI, there are a number of issues already addressed in bionic arms, which can enhance the adoption of exoskeleton technologies. Effortless donning and doffing of an external device can have a positive effect on a user's satisfaction and presents an aspect already well-studied for bionic arms. Moreover, cosmetic gloves and artificial skin ensure a natural appearance and thus enhance the acceptability of such devices. Exoskeletons can benefit from the successful examples already set for bionic arms. The fact that amputees may have specific surgeries performed to improve fit (like osseointegration) or bionic arm control (like TMR) suggests that surgical procedures could become available for individuals using exoskeletons. Such procedures could also restore sensory feedback in people with Stroke or DMD, when impaired, similar to what is done for amputees [119]. This is important for the upper limb, as the sense of touch and proprioception is central for object manipulation [120]. Additionally, the restoration of sensory feedback enables natural closed-loop control (Section III) and improves fine motor control in terms of coordination and dexterity [121]–[123]. However, it is important to consider that while amputees might have

the level of commitment to consider invasive surgery, paretic patients or muscular dystrophy patients may not have it. In these neurological conditions, it is not uncommon that sensory feedback and proprioception may be restored through non-invasive ways, such as rehabilitation [124] or that are not even impaired [103], [125].

V. CONCLUSION

A focused perspective on the development of personalised HMI schemes to enhance upper extremity function via robotic exoskeletons, is discussed for the cases of stroke and DMD. We believe that the use of the proposed schemes can help the development of better HMI schemes for users of robotic exoskeletons of the upper limb, enhance function and daily use of such devices, and inspire more research towards the development of hybrid HMI.

ACKNOWLEDGMENT

The authors would like to thank Arvid Q. L. Keemink for his insightful comments regarding the proposed control schemes.

REFERENCES

- [1] R. Morris and I. Q. Whishaw, "Arm and hand movement: Current knowledge and future perspective," *Front. Neurol.*, vol. 6, p. 19, Feb. 2015.
- [2] A. Basteris *et al.*, "Training modalities in robot-mediated upper limb rehabilitation in stroke: A framework for classification based on a systematic review," *J. Neuroeng. Rehabil.*, vol. 11, no. 1, p. 111, 2014.
- [3] R. A. Bos *et al.*, "A structured overview of trends and technologies used in dynamic hand orthoses," *J. Neuroeng. Rehabil.*, vol. 13, no. 1, p. 62, 2016.
- [4] F. Sergi, A. Blank, and M. O'Malley, "Upper extremity exoskeleton for robot-aided rehabilitation," *Mech. Eng. Mag. Sel. Articles*, vol. 136, no. 9, pp. S6–S11, Sep. 2014.
- [5] H. Fritz, D. Patzer, and S. S. Galen, "Robotic exoskeletons for re-gaging in everyday activities: Promises, pitfalls, and opportunities," *Disability Rehabil.*, vol. 41, no. 5, pp. 560–563, 2017.
- [6] S. Demain *et al.*, "Assistive technologies after stroke: Self-management or fending for yourself? A focus group study," *BMC Health Services Res.*, vol. 13, p. 334, Aug. 2013.
- [7] P. P. Maciejasz, J. Eschweiler, K. Gerlach-Hahn, A. Jansen-Troy, and S. Leonhardt, "A survey on robotic devices for upper limb rehabilitation," *J. Neuroeng. Rehabil.*, vol. 11, p. 3, Jan. 2014.
- [8] D. J. Reinkensmeyer and M. L. Boninger, "Technologies and combination therapies for enhancing movement training for people with a disability," *J. Neuroeng. Rehabil.*, vol. 9, no. 1, p. 17, 2012.
- [9] M. Xiloyannis, D. Chiaradia, A. Frisoli, and L. Masia, "Physiological and kinematic effects of a soft exosuit on arm movements," *J. Neuroeng. Rehabil.*, vol. 16, no. 1, p. 29, 2019.
- [10] C. T. O'Neill, N. S. Phipps, L. Cappello, S. Paganoni, and C. J. Walsh, "A soft wearable robot for the shoulder: Design, characterization, and preliminary testing," in *Proc. IEEE Int. Conf. Rehabil. Robot.*, 2017, pp. 1672–1678.
- [11] T. Proietti, V. Crocher, A. Roby-Brami, and N. Jarrassé, "Upper-limb robotic exoskeletons for neurorehabilitation: A review on control strategies," *IEEE Rev. Biomed. Eng.*, vol. 9, pp. 4–14, 2016.
- [12] T. G. Hornby *et al.*, "Enhanced gait-related improvements after therapist-versus robotic-assisted locomotor training in subjects with chronic stroke: A randomized controlled study," *Stroke*, vol. 39, no. 6, pp. 1786–1792, 2008.
- [13] F. Amirabdollahian *et al.*, "Design, development and deployment of a hand/wrist exoskeleton for home-based rehabilitation after stroke—SCRIPT project," *Robotica*, vol. 32, no. 8, pp. 1331–1346, Dec. 2014.
- [14] S. Ates, J. Lobo-Prat, P. Lammertse, H. Van Der Kooij, and A. H. A. Stienen, "SCRIPT passive orthosis: Design and technical evaluation of the wrist and hand orthosis for rehabilitation training at home," in *Proc. IEEE Int. Conf. Rehabil. Robot.*, Seattle, WA, USA, 2013, pp. 1–6.
- [15] J. Laut, M. Porfiri, and P. Raghavan, "The present and future of robotic technology in rehabilitation," *Current Phys. Med. Rehabil. Rep.*, vol. 4, no. 4, pp. 312–319, 2016.
- [16] F. Yakub, A. Z. M. Khudzari, and Y. Mori, "Recent trends for practical rehabilitation robotics, current challenges and the future," *Int. J. Rehabil. Res.*, vol. 37, no. 1, pp. 9–21, 2014.
- [17] *Improving the Human-Machine Interface: Revolutionary Advancements in Upper-Limb Prostheses*. Accessed: Nov. 20, 2018. [Online]. Available: <https://lopedge.com>
- [18] J. S. Hebert, K. Elzinga, K. M. Chan, J. Olson, and M. Morhart, "Updates in targeted sensory reinnervation for upper limb amputation," *Current Surgery Rep.*, vol. 2, no. 3, p. 45, Mar. 2014.
- [19] M. Sartori, U. Ş. Yavuz, and D. Farina, "In vivo neuromechanics: Decoding causal motor neuron behavior with resulting musculoskeletal function," *Sci. Rep.*, vol. 7, no. 1, 2017, Art. no. 13465.
- [20] S. Jönsson, K. Caine-Winterberger, and R. Branemark, "Osseointegration amputation prostheses on the upper limbs: Methods, prosthetics and rehabilitation," *Prosthet. Orthot. Int.*, vol. 35, no. 2, pp. 190–200, 2011.
- [21] O. C. Aszmann *et al.*, "Elective amputation and bionic substitution restore functional hand use after critical soft tissue injuries," *Sci. Rep.*, vol. 6, Oct. 2016, Art. no. 34960.
- [22] *MyoPro Elbow-Wrist-Hand Orthosis (EWHO)*. Accessed: Apr. 8, 2019. [Online]. Available: <https://myomo.com/what-is-a-myopro-orthosis/>
- [23] G. J. Kim, L. Rivera, and J. Stein, "Combined clinic-home approach for upper limb robotic therapy after stroke: A pilot study," *Archives Phys. Med. Rehabil.*, vol. 96, no. 12, pp. 2243–2248, 2015.
- [24] *SaeboGlove—Finger Extension Rehabilitation Glove for Stroke Survivors*. Accessed: Apr. 8, 2019. [Online]. Available: <https://www.saebo.com/saeboglove/>
- [25] C. Sherstan, "Towards prosthetic arms as wearable intelligent robots," Ph.D. dissertation, Univ. Alberta, Edmonton, AB, Canada, 2015, p. 150.
- [26] *COAPT*. Accessed: Apr. 8, 2019. [Online]. Available: <https://www.coaptengineering.com/>
- [27] *Empower—Ottobock U.S.* Accessed: Apr. 8, 2019. [Online]. Available: <https://www.ottobock.com/prosthetics/lower-limb-prosthetics/solution-overview/empower-ankle/>
- [28] K. Norton, "A brief history of prosthetics," *inMotion*, vol. 17, no. 7, pp. 11–13, 2007.
- [29] L. J. Marks and J. W. Michael, "Science, medicine, and the future: Artificial limbs," *BMJ*, vol. 323, no. 7315, pp. 732–735, 2001.
- [30] N. M. Maleševič *et al.*, "A multi-pad electrode based functional electrical stimulation system for restoration of grasp," *J. Neuroeng. Rehabil.*, vol. 9, no. 1, p. 66, 2012.
- [31] L. P. Popovič-Maneski *et al.*, "Multi-pad electrode for effective grasping: Design," *IEEE Trans. Neural Syst. Rehabil. Eng.*, vol. 21, no. 4, pp. 648–654, Jul. 2013.
- [32] N. Jiang, H. Rehbaum, I. Vujaklija, B. Graitmann, and D. Farina, "Intuitive, online, simultaneous, and proportional myoelectric control over two degrees-of-freedom in upper limb amputees," *IEEE Trans. Neural Syst. Rehabil. Eng.*, vol. 22, no. 3, pp. 501–510, May 2014.
- [33] N. Jiang, J. L. Vest-Nielsen, S. Muceli, and D. Farina, "EMG-based simultaneous and proportional estimation of wrist/hand dynamics in uni-lateral trans-radial amputees," *J. Neuroeng. Rehabil.*, vol. 9, no. 1, p. 42, 2012.
- [34] E. J. Rouse, N. C. Villagaray-Carski, R. W. Emerson, and H. M. Herr, "Design and testing of a bionic dancing prosthesis," *PLoS ONE*, vol. 10, no. 8, pp. 1–6, 2015.
- [35] G. Aguirre-Ollinger, J. E. Colgate, M. A. Peshkin, and A. Goswami, "Active-impedance control of a lower-limb assistive exoskeleton," in *Proc. IEEE 10th Int. Conf. Rehabil. Robot. (ICORR)*, 2007, pp. 188–195.
- [36] G. Smit, D. H. Plettenburg, and F. C. T. T. Van Der Helm, "The lightweight delft cylinder hand: First multi-articulating hand that meets the basic user requirements," *IEEE Trans. Neural Syst. Rehabil. Eng.*, vol. 23, no. 3, pp. 431–440, May 2015.
- [37] L. Haverkate, G. Smit, and D. H. Plettenburg, "Assessment of body-powered upper limb prostheses by able-bodied subjects, using the box and blocks test and the nine-hole peg test," *Prosthet. Orthot. Int.*, vol. 40, no. 1, pp. 109–116, 2016.
- [38] T. Rahman *et al.*, "Design and testing of a functional arm orthosis in patients with neuromuscular diseases," *IEEE Trans. Neural Syst. Rehabil. Eng.*, vol. 15, no. 2, pp. 244–251, Jun. 2007.
- [39] J. Lobo-Prat *et al.*, "Implementation of EMG- and force-based control interfaces in active elbow supports for men with duchenne muscular dystrophy: A feasibility study," *IEEE Trans. Neural Syst. Rehabil. Eng.*, vol. 24, no. 11, pp. 1179–1190, Nov. 2016.

- [40] C. L. Jones, F. Wang, R. Morrison, N. Sarkar, and D. G. Kamper, "Design and development of the cable actuated finger exoskeleton for hand rehabilitation following stroke," *IEEE/ASME Trans. Mechatronics*, vol. 19, no. 1, pp. 131–140, Feb. 2014.
- [41] J. M. Ochoa, D. G. Kamper, M. Listenberger, and S. W. Lee, "Use of an electromyographically driven hand orthosis for training after stroke," in *Proc. IEEE Int. Conf. Rehabil. Robot.*, Zürich, Switzerland, 2011, pp. 1–5.
- [42] J. Lobo-Prat *et al.*, "Non-invasive control interfaces for intention detection in active movement-assistive devices," *J. Neuroeng. Rehabil.*, vol. 11, no. 1, p. 168, 2014.
- [43] B. R. Wittenauer and L. Smith, *Background Paper 6. 6 Ischaemic and Haemorrhagic Stroke: Priority Medicines for Europe and the World a Public Health Approach to Innovation*, WHO, Geneva, Switzerland, Dec. 2012.
- [44] K. J. Nowak and K. E. Davies, "Duchenne muscular dystrophy and dystrophin: Pathogenesis and opportunities for treatment: Third in molecular medicine review series," *EMBO Rep.*, vol. 5, no. 9, pp. 872–876, 2004.
- [45] A. G. Thrift *et al.*, "Global stroke statistics," *Int. J. Stroke*, vol. 12, no. 1, pp. 13–32, 2017.
- [46] A. Cosh and H. Carslaw, "Multiple sclerosis: Symptoms and diagnosis," *Innovait Educ. Inspiration Gen. Pract.*, vol. 7, no. 11, pp. 651–657, 2014.
- [47] K. Nas, L. Yazmalar, V. Şah, A. Aydın, and K. Öneş, "Rehabilitation of spinal cord injuries," *World J. Orthopedics*, vol. 6, no. 1, pp. 8–16, 2015.
- [48] V. Dietz and T. Sinkjaer, "Spastic movement disorder: Impaired reflex function and altered muscle mechanics," *Lancet Neurol.*, vol. 6, no. 8, pp. 725–733, 2007.
- [49] C. Adrienne and C. Manigandan, "Inpatient occupational therapists hand-splinting practice for clients with stroke: A cross-sectional survey from Ireland," *J. Neurosci. Rural Pract.*, vol. 2, no. 2, pp. 141–149, 2011.
- [50] N. A. Lannin and R. D. Herbert, "Is hand splinting effective for adults following stroke? A systematic review and methodological critique of published research," *Clin. Rehabil.*, vol. 17, no. 8, pp. 807–816, 2003.
- [51] A. Andringa, I. van de Port, and J.-W. Meijer, "Long-term use of a static hand-wrist orthosis in chronic stroke patients: A pilot study," *Stroke Res. Treat.*, vol. 2013, Feb. 2013, Art. no. 546093.
- [52] A. Duschau-Wicke, A. Caprez, and R. Rienen, "Patient-cooperative control increases active participation of individuals with SCI during robot-aided gait training," *J. Neuroeng. Rehabil.*, vol. 7, no. 1, p. 43, 2010.
- [53] S. Srivastava *et al.*, "Robotic assist-as-needed as an alternative to therapist-assisted gait rehabilitation," *Int. J. Phys. Med. Rehabil.*, vol. 4, no. 5, p. 370, 2016.
- [54] B. Bartels *et al.*, "Upper limb function in adults with Duchenne muscular dystrophy," *J. Rehabil. Med.*, vol. 43, no. 9, pp. 770–775, 2011.
- [55] M. Eagle *et al.*, "Survival in Duchenne muscular dystrophy: Improvements in life expectancy since 1967 and the impact of home nocturnal ventilation," *Neuromuscul. Disord.*, vol. 12, no. 10, pp. 926–929, 2002.
- [56] K. R. Wagner, N. Lechtzin, and D. P. Judge, "Current treatment of adult Duchenne muscular dystrophy," *Biochim. Biophys. Acta*, vol. 1772, no. 2, pp. 229–237, 2007.
- [57] B. T. Darras, D. T. Miller, and D. K. Urion, "Dystrophinopathies," in *GeneReviews®*, R. A. Pagon *et al.*, Eds. Seattle, WA, USA: Univ. Washington, 2016. Accessed: Feb. 21, 2017. [Online]. Available: <http://www.ncbi.nlm.nih.gov/books/NBK11119/>
- [58] S. L. Houwen-van Opstal, M. Jansen, N. van Alfen, and I. J. M. de Groot, "Health-related quality of life and its relation to disease severity in boys with duchenne muscular dystrophy: Satisfied boys, worrying parents—A case-control study," *J. Child Neurol.*, vol. 29, no. 11, pp. 1486–1495, 2013.
- [59] M. B. Wagner, P. J. Vignos, and C. Carozzi, "Duchenne muscular dystrophy: A study of wrist and hand function," *Muscle Nerve*, vol. 12, no. 3, pp. 236–244, 1989.
- [60] A. Bergsma *et al.*, "1st workshop on upper-extremity assistive technology for people with duchenne: State of the art, emerging avenues, and challenges. April 27th 2015, London, United Kingdom," *Neuromuscul. Disord.*, vol. 26, no. 6, pp. 386–393, 2016.
- [61] M. M. Janssen, A. Bergsma, A. C. H. Geurts, and I. J. M. De Groot, "Patterns of decline in upper limb function of boys and men with DMD: An international survey," *J. Neurol.*, vol. 261, no. 7, pp. 1269–1288, 2014.
- [62] J. Weichbrodt, B.-M. Eriksson, and A.-K. Kroksmark, "Evaluation of hand orthoses in Duchenne muscular dystrophy," *Disability Rehabil.*, vol. 40, no. 23, pp. 2824–2832, 2018.
- [63] P. Geethanjali, "Myoelectric control of prosthetic hands: State-of-the-art review," *Med. Devices Evidence Res.*, vol. 9, pp. 247–255, Jul. 2016.
- [64] D. Farina and M. Sartori, "Surface electromyography for MAN-machine interfacing in rehabilitation technologies," in *Surface Electromyography Physiology, Engineering and Applications*. New York, NY, USA: Wiley, 2016, pp. 540–560.
- [65] A. Fougner, O. Stavadahl, P. J. Kyberd, Y. G. Losier, and P. A. Parker, "Control of upper limb prostheses: Terminology and proportional myoelectric control—A review," *IEEE Trans. Neural Syst. Rehabil. Eng.*, vol. 20, no. 5, pp. 663–677, Sep. 2012.
- [66] F. J. Valero-Cuevas, H. Hoffmann, M. U. Kurse, J. J. Kutch, and E. A. Theodorou, "Computational models for neuromuscular function," *IEEE Rev. Biomed. Eng.*, vol. 2, pp. 110–135, 2009.
- [67] J. Yousefi and A. Hamilton-Wright, "Characterizing EMG data using machine-learning tools," *Comput. Biol. Med.*, vol. 51, pp. 1–13, Aug. 2014.
- [68] M. Sartori, D. G. Llyod, and D. Farina, "Neural data-driven musculoskeletal modeling for personalized neurorehabilitation technologies," *IEEE Trans. Biomed. Eng.*, vol. 63, no. 5, pp. 879–893, May 2016.
- [69] G. Durandau, D. Farina, and M. Sartori, "Robust real-time musculoskeletal modeling driven by electromyograms," *IEEE Trans. Biomed. Eng.*, vol. 65, no. 3, pp. 556–564, May 2018.
- [70] M. Sartori, G. Durandau, S. Došen, and D. Farina, "Robust simultaneous myoelectric control of multiple degrees of freedom in wrist-hand prostheses by real-time neuromusculoskeletal modeling," *J. Neural Eng.*, vol. 15, no. 6, 2018, Art. no. 066026.
- [71] M. Sartori, J. van de Riet, and D. Farina, "Estimation of phantom arm mechanics about four degrees of freedom after targeted muscle reinnervation," *IEEE Trans. Med. Robot. Bionics*, vol. 1, no. 1, pp. 58–64, Feb. 2019.
- [72] M. Atzori and H. Müller, "Control capabilities of myoelectric robotic prostheses by hand amputees: A scientific research and market overview," *Front. Syst. Neurosci.*, vol. 9, pp. 1–7, Nov. 2015.
- [73] S. Muceli and D. Farina, "Simultaneous and proportional estimation of hand kinematics from EMG during mirrored movements at multiple degrees-of-freedom," *IEEE Trans. Neural Syst. Rehabil. Eng.*, vol. 20, no. 3, pp. 371–378, May 2012.
- [74] N. Jiang, S. Dosen, K. R. Muller, and D. Farina, "Myoelectric control of artificial limbs: Is there a need to change focus? [in the spotlight]," *IEEE Signal Process. Mag.*, vol. 29, no. 5, pp. 150–152, Sep. 2012.
- [75] M. Ison and P. Artemiadis, "The role of muscle synergies in myoelectric control: Trends and challenges for simultaneous multifunction control," *J. Neural Eng.*, vol. 11, no. 5, 2014, Art. no. 051001.
- [76] K. S. Türker, "Electromyography: Some methodological problems and issues," *Phys. Ther.*, vol. 73, no. 10, pp. 698–710, 1993.
- [77] A. Chadwell, L. Kenney, S. Thies, A. Galpin, and J. Head, "The reality of myoelectric prostheses: Understanding what makes these devices difficult for some users to control," *Front. Neurobot.*, vol. 10, p. 7, Aug. 2016.
- [78] N. Hogan, "Impedance control: An approach to manipulation: Part III—Applications," *J. Dyn. Syst. Meas. Control*, vol. 107, no. 1, pp. 17–24, 1985.
- [79] S. K. Au and H. M. Herr, "Powered ankle-foot prosthesis," *IEEE Robot. Autom. Mag.*, vol. 15, no. 3, pp. 52–59, Sep. 2008.
- [80] E. J. Rouse, L. M. Mooney, and H. M. Herr, "Clutchable series-elastic actuator: Implications for prosthetic knee design," *Int. J. Robot. Res.*, vol. 33, no. 13, pp. 1611–1625, 2014.
- [81] B. E. Lawson *et al.*, "A robotic leg prosthesis: Design, control, and implementation," *Robot. Autom. Mag.*, vol. 21, no. 4, pp. 70–81, Dec. 2014.
- [82] M. Goldfarb, B. E. Lawson, and A. H. Shultz, "Realizing the promise of robotic leg prostheses," *Sci. Transl. Med.*, vol. 5, no. 210, 2013, Art. no. 210ps15.
- [83] A. J. Young, L. H. Smith, E. J. Rouse, and L. J. Hargrove, "Classification of simultaneous movements using surface EMG pattern recognition," *IEEE Trans. Biomed. Eng.*, vol. 60, no. 5, pp. 1250–1258, May 2013.
- [84] P. Parker, K. Englehart, and B. Hudgins, "Myoelectric signal processing for control of powered limb prostheses," *J. Electromyography Kinesiol.*, vol. 16, no. 6, pp. 541–548, 2006.

- [85] A. Q. L. Keemink, H. van der Kooij, and A. H. A. Stienen, "Admittance control for physical human-robot interaction," *Int. J. Robot. Res.*, vol. 37, no. 11, pp. 1421-1444, 2018.
- [86] N. Wiener, *Cybernetics: Control and Communication in the Animal and the Machine*, 2nd ed. Cambridge, MA, USA: MIT Press, 1961, p. 212.
- [87] R. F. Weir, C. W. Heckathorne, and D. S. Childress, "Cineplasty as a control input for externally powered prosthetic components," *J. Rehabil. Res. Dev.*, vol. 38, no. 4, pp. 357-363, 2001.
- [88] W. Craelius, "The bionic man: Restoring mobility," *Science*, vol. 295, no. 5557, pp. 1018-1021, 2002.
- [89] J. Silva, W. Heim, and T. Chau, "A self-contained, mechanomyography-driven externally powered prosthesis," *Archives Phys. Med. Rehabil.*, vol. 86, no. 10, pp. 2066-2070, 2005.
- [90] S. Micera *et al.*, "Decoding of grasping information from neural signals recorded using peripheral intrafascicular interfaces," *J. Neuroeng. Rehabil.*, vol. 8, no. 1, p. 53, 2011.
- [91] K. Ohnishi, R. F. Weir, and T. A. Kuiken, "Neural machine interfaces for controlling multifunctional powered upper-limb prostheses," *Expert Rev. Med. Devices*, vol. 4, no. 1, pp. 43-53, 2007.
- [92] R. A. Bruinekool and I. D. H. Plettenburg, "Pneumatic pinch force magnification in voluntary closing hand prostheses," M.S. thesis, Dept. Biomech. Eng., TU-Delft, Delft, The Netherlands, Sep. 2012.
- [93] H. Ring and N. Rosenthal, "Controlled study of neuroprosthetic functional electrical stimulation in sub-acute post-stroke rehabilitation," *J. Rehabil. Med.*, vol. 37, no. 1, pp. 32-36, 2005.
- [94] G. E. Loeb, R. A. Peck, W. H. Moore, and K. Hood, "BIONTM system for distributed neural prosthetic interfaces," *Med. Eng. Phys.*, vol. 23, no. 1, pp. 9-18, 2001.
- [95] R. Turk *et al.*, "Therapeutic effectiveness of electric stimulation of the upper-limb poststroke using implanted microstimulators," *Archives Phys. Med. Rehabil.*, vol. 89, no. 10, pp. 1913-1922, 2008.
- [96] M. W. Keith *et al.*, "Implantable functional neuromuscular stimulation in the tetraplegic hand," *J. Hand Surg. Amer.*, vol. 14, no. 3, pp. 524-530, 1989.
- [97] S. Mazzoleni, C. Duret, A. G. Grosmaire, and E. Battini, "Combining upper limb robotic rehabilitation with other therapeutic approaches after stroke: Current status, rationale, and challenges," *Biomed Res. Int.*, vol. 2017, Sep. 2017, Art. no. 8905637.
- [98] S.-H. Moon, J.-H. Choi, and S.-E. Park, "The effects of functional electrical stimulation on muscle tone and stiffness of stroke patients," *J. Phys. Ther. Sci.*, vol. 29, no. 2, pp. 238-241, 2017.
- [99] S. P. Sayers, "The role of exercise as a therapy for children with duchenne muscular dystrophy," *Pediatr. Exercise Sci.*, vol. 12, pp. 23-33, Feb. 2000.
- [100] P. A. Parker and R. N. Scott, "Myoelectric control of prostheses," *Crit. Rev. Biomed. Eng.*, vol. 13, no. 4, pp. 283-310, 1986.
- [101] A. Zupan, "Long-term electrical stimulation of muscles in children with duchenne and Becker muscular dystrophy," *Muscle Nerve*, vol. 15, no. 3, pp. 362-367, 1992.
- [102] T. Ansved, "Muscular dystrophies: Influence of physical conditioning on the disease evolution," *Current Opin. Clin. Nutr. Metab. Care*, vol. 6, no. 4, pp. 435-439, 2003.
- [103] D. Rand, "Proprioception deficits in chronic stroke-upper extremity function and daily living," *PLoS ONE*, vol. 13, no. 3, 2018, Art. no. e0195043.
- [104] S. Yao, Y. Zhuang, Z. Li, and R. Song, "Adaptive admittance control for an ankle exoskeleton using an EMG-driven musculoskeletal model," *Front. Neurobot.*, vol. 12, p. 16, Apr. 2018.
- [105] J. Lobo-Prat *et al.*, "Adaptive gravity and joint stiffness compensation methods for force-controlled arm supports," in *Proc. IEEE Int. Conf. Rehabil. Robot. (ICORR)*, vol. 2, 2015, pp. 478-483.
- [106] J. Lobo-Prat *et al.*, "Comparison between SEMG and force as control interfaces to support planar arm movements in adults with Duchenne: A feasibility study," *J. Neuroeng. Rehabil.*, vol. 14, no. 1, pp. 1-17, 2017.
- [107] Y. Hara, "Neurorehabilitation with new functional electrical stimulation for hemiparetic upper extremity in stroke patients," *J. Nippon Med. Sch.*, vol. 75, no. 1, pp. 4-14, 2008.
- [108] P. Krause, J. Szecsi, and A. Straube, "Changes in spastic muscle tone increase in patients with spinal cord injury using functional electrical stimulation and passive leg movements," *Clin. Rehabil.*, vol. 22, no. 7, pp. 627-634, 2008.
- [109] P. Krause, J. Szecsi, and A. Straube, "FES cycling reduces spastic muscle tone in a patient with multiple sclerosis," *NeuroRehabilitation*, vol. 22, no. 4, pp. 335-337, 2007.
- [110] D. Skuk, M. Goulet, and J. P. Tremblay, "Preservation of muscle spindles in a 27-year-old Duchenne muscular dystrophy patient: Importance for regenerative medicine strategies," *Muscle Nerve*, vol. 41, no. 5, pp. 729-730, 2010.
- [111] J. Lobo-Prat *et al.*, "Evaluation of EMG, force and joystick as control interfaces for active arm supports," *J. Neuroeng. Rehabil.*, vol. 11, p. 68, Apr. 2014.
- [112] M. Sartori *et al.*, "Toward modeling locomotion using electromyography-informed 3D models: Application to cerebral palsy," *Interdiscip. Rev. Syst. Biol. Med.*, vol. 9, no. 2, Mar. 2017, Art. no. e1368.
- [113] J. Fernandez *et al.*, "Multiscale musculoskeletal modelling, data-model fusion and electromyography-informed modeling," *Interface Focus*, vol. 6, no. 2, 2016, Art. no. 20150084.
- [114] J. A. Franck, R. J. E. M. Smeets, and H. A. M. Seelen, "Evaluation of a functional hand orthosis combined with electrical stimulation adjunct to arm-hand rehabilitation in subacute stroke patients with a severely to moderately affected hand function," *Disability Rehabil.*, vol. 9, pp. 1-9, Jan. 2018.
- [115] J. Ribeiro *et al.*, "Analysis of man-machine interfaces in upper-limb prosthesis: A review," *Robotics*, vol. 8, no. 1, p. 16, 2019.
- [116] J. Gancet *et al.*, "MINDWALKER: Going one step further with assistive lower limbs exoskeleton for SCI condition subjects," in *Proc. IEEE RAS EMBS Int. Conf. Biomed. Robot. Biomechatron.*, 2012, pp. 1794-1800.
- [117] T. Misawa, K. Goto, S. Takano, and S. Hirobayashi, "A development of NIRS-based brain-computer interface for robot control," *IEEJ Trans. Sensors Micromach.*, vol. 132, no. 10, pp. 355-361, Oct. 2012.
- [118] J. Shi, Q. Chang, and Y.-P. Zheng, "Feasibility of controlling prosthetic hand using sonomyography signal in real time: Preliminary study," *J. Rehabil. Res. Dev.*, vol. 47, no. 2, pp. 87-98, 2010.
- [119] P. Svensson, U. Wijk, A. Björkman, and C. Antfolk, "A review of invasive and non-invasive sensory feedback in upper limb prostheses," *Exp. Rev. Med. Devices*, vol. 14, no. 6, pp. 439-447, 2017.
- [120] R. S. Johansson and J. R. Flanagan, "Coding and use of tactile signals from the fingertips in object manipulation tasks," *Nat. Rev. Neurosci.*, vol. 10, no. 5, pp. 345-359, 2009.
- [121] D. W. Tan *et al.*, "A neural interface provides long-term stable natural touch perception," *Sci. Transl. Med.*, vol. 6, no. 257, 2014, Art. no. 257ra138.
- [122] F. M. Petrini *et al.*, "Six-month assessment of a hand prosthesis with intraneural tactile feedback," *Ann. Neurol.*, vol. 85, no. 1, pp. 137-154, 2019.
- [123] F. Clemente *et al.*, "Intraneural sensory feedback restores grip force control and motor coordination while using a prosthetic hand," *J. Neural Eng.*, vol. 16, no. 2, 2019, Art. no. 026034.
- [124] N. Bolognini, C. Russo, and D. J. Edwards, "The sensory side of post-stroke motor rehabilitation," *Restor. Neurol. Neurosci.*, vol. 34, no. 4, pp. 571-586, 2016.
- [125] E. Ribot-Ciscar *et al.*, "Is muscle spindle proprioceptive function spared in muscular dystrophies? A muscle tendon vibration study," *Muscle Nerve*, vol. 29, no. 6, pp. 861-866, 2004.